The measurement of induction shocks: a manual for the quantitative use of Faradic stimuli / by Ernest G. Martin.

Contributors

Martin, Ernest Gale, 1876-1934. Augustus Long Health Sciences Library

Publication/Creation

New York: J. Wiley & Sons; [etc., etc.], 1912.

Persistent URL

https://wellcomecollection.org/works/v23abmr3

License and attribution


This material has been provided by This material has been provided by the Augustus C. Long Health Sciences Library at Columbia University and Columbia University Libraries/Information Services, through the Medical Heritage Library. The original may be consulted at the the Augustus C. Long Health Sciences Library at Columbia University and Columbia University. where the originals may be consulted.

This work has been identified as being free of known restrictions under copyright law, including all related and neighbouring rights and is being made available under the Creative Commons, Public Domain Mark.

You can copy, modify, distribute and perform the work, even for commercial purposes, without asking permission.



Wellcome Collection
183 Euston Road
London NW1 2BE UK
T +44 (0)20 7611 8722
E library@wellcomecollection.org
https://wellcomecollection.org

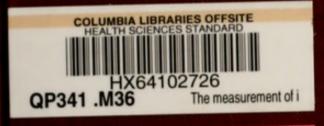

RECAP

Columbia University Cop.1. inthe City of New York


College of Physicians and Surgeons




Reference Library


Given by

IV. P. Burron-Opira.

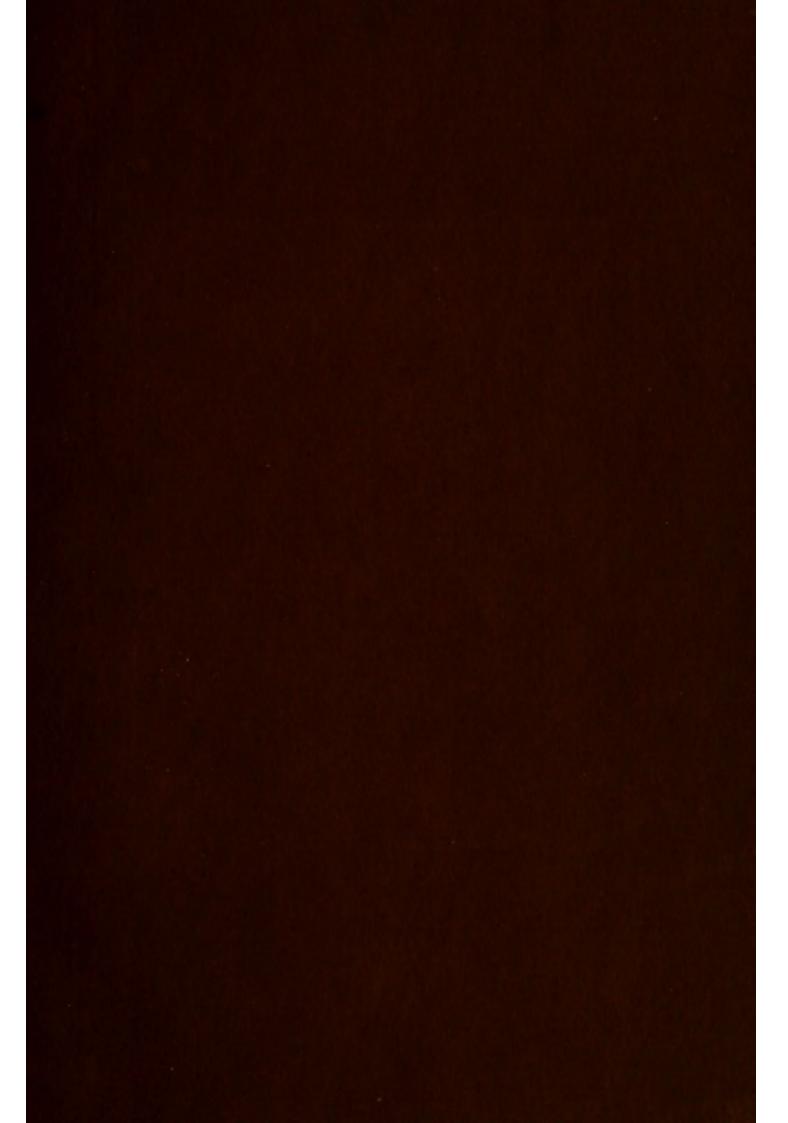

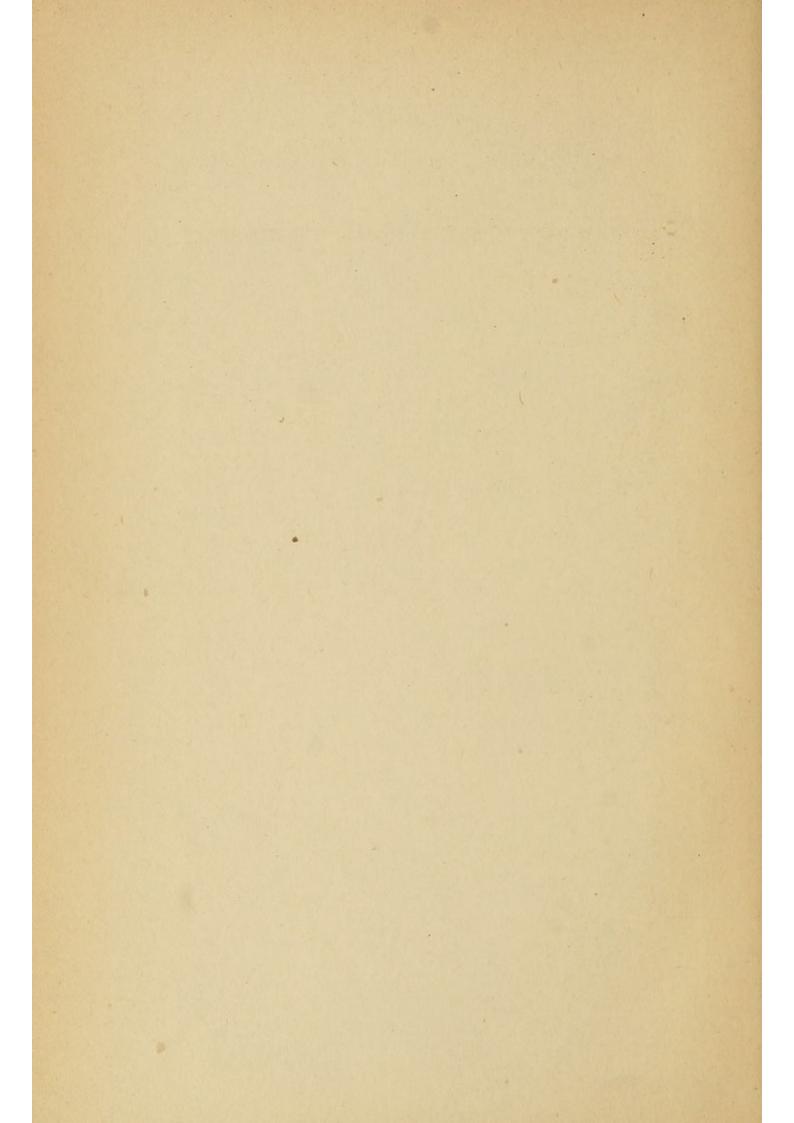

Digitized by the Internet Archive in 2010 with funding from Columbia University Libraries

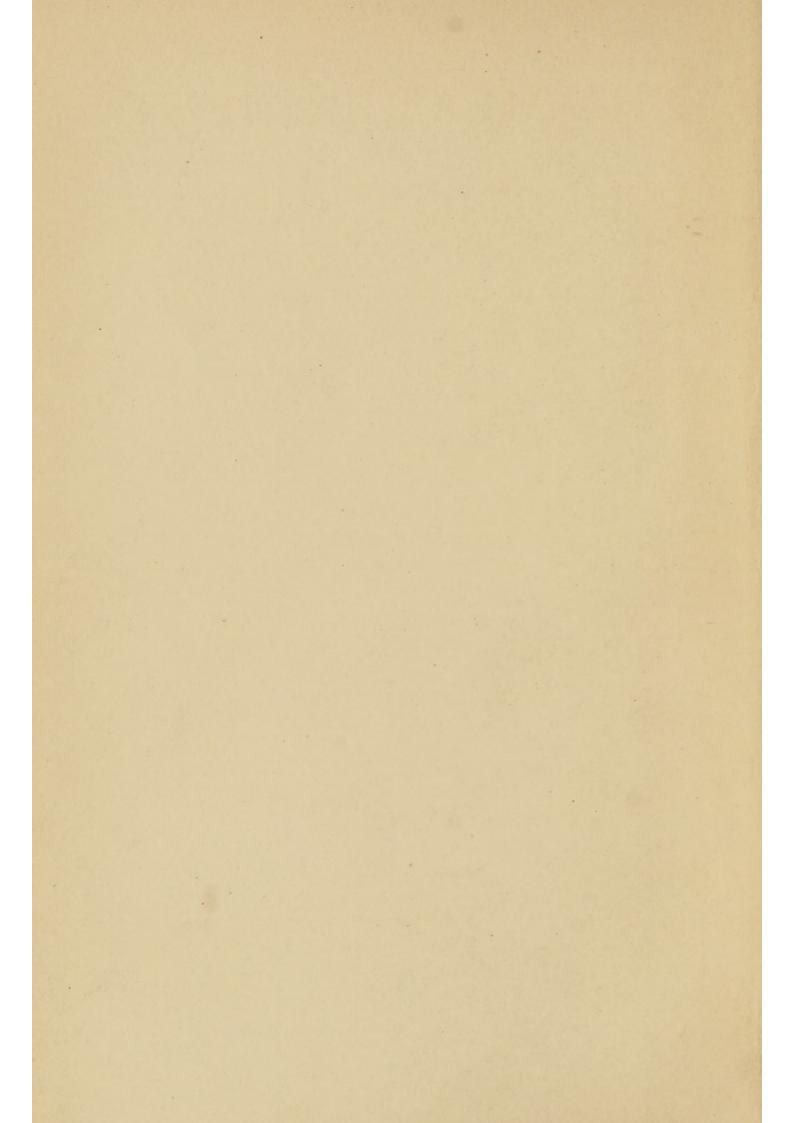

THE MEASUREMENT OF INDUCTION SHOCKS

A MANUAL FOR THE QUANTITATIVE
USE OF FARADIC STIMULI

BY

ERNEST G. MARTIN, Ph. D.

ASSISTANT PROFESSOR OF PHYSIOLOGY IN THE HARVARD MEDICAL SCHOOL

FIRST EDITION
FIRST THOUSAND

NEW YORK

JOHN WILEY & SONS

LONDON: CHAPMAN & HALL, LIMITED

1912

COPYRIGHT. 1912,
BY
ERNEST G. MARTIN

Stanbope Press

F. H. GILSON COMPANY BOSTON, U.S.A.

PREFATORY NOTE

The method of measuring induction shocks described in the following pages was developed in a series of papers published between 1908 and 1911 in the American Journal of Physiology. Extended use of the method by myself and coworkers has shown it to have great value in many physiological and psychological researches. In order to make the method more readily available for investigators, and with the hope that thereby quantitative studies may be more generally made, the scattered material of the original papers has been assembled into the form herein presented. Since the work aims to serve rather as a manual than as an exposition of principles, only so much theoretical matter is included as is necessary to make intelligible the procedures adopted.

E. G. M.

BOSTON, April, 1912.



CONTENTS

CHAPTER I.	_
	PAGE
THE CHARACTERISTICS OF INDUCED CURRENTS	I
Introductory	I
Historical	2
Structure of the Inductorium	3
Principle of the Inductorium	4
The Form of Make and Break Induced Currents	8
CHAPTER II.	
FACTORS WHICH AFFECT THE STRENGTHS OF FARADIC STIMULI	12
Sources of Variation	13
Methods Previously Proposed	14
Pflüger	14
Meyer-Fick	15
Kronecker	16
v. Fleischl	18
Wertheim-Salomonson	18
Edelmann	20
Hoorweg-Giltay	21
CHAPTER III.	
A SUMMARY OF PROCEDURE	23
Instruments Required for the Calibration	23
Ammeter and Shunt	24
Stimulating Electrodes	27
n 1	-0

CHAPTER IV.	PAGE
THE PHYSICAL PRINCIPLES UNDERLYING THE MEASUREMENT OF	PAGE
Break Shocks	32
The Course of Break Induced Currents	32
CHAPTER V.	
THE DETERMINATIONS OF MUTUAL INDUCTION BETWEEN PRIMARY AND SECONDARY COILS	38
CHAPTER VI.	
Effects Produced by an Iron Core in the Primary Coil	43
CHAPTER VII.	
Comparison of One Coil with Another — The Value of $L\dots$	50
CHAPTER VIII.	
THE PREPARATION OF A CALIBRATION SCALE FOR BREAK SHOCKS	55
CHAPTER IX.	
THE MAKE AND BREAK OF THE PRIMARY CIRCUIT	60
The Knife-blade Key	63
The Operating Device	65
The Short-circuiting Device	67
CHAPTER X.	
THE INFLUENCE OF SECONDARY RESISTANCE AND OF CATHODE	
Surface	71
The Relation of Tissue Resistance to Secondary Resistance as a Whole	
Determination of Tissue Resistance	-
Effect upon the Stimulus of Varying the Secondary Resistance	73
Current Density, an Important Factor	76

CONTENTS	vii
CHAPTER X — Continued.	
	PAGE
The Dependence of Factor A upon Inductorium Construction Conditions in which the Specific Stimulus need not be De-	78
termined	80
A Standard of Inductorium Construction Necessary	88
CHAPTER XI.	
THE MEASUREMENT OF MAKE SHOCKS	94
Stimuli	99
CHAPTER XII.	
Errors to be Avoided	107



INDUCTION SHOCKS

CHAPTER I

THE CHARACTERISTICS OF INDUCED CURRENTS

Introductory. The inductorium has become one of the most familiar and most useful instruments in the physiological laboratory. There are few physiological researches which do not involve artificial stimulation of tissues; and for the production of stimuli induction shocks are in most cases the first choice. They are easier to use and they subject the stimulated tissue to less permanent modification than do other forms of artificial stimulus. Induction shocks are, however, very variable in intensity; and as commonly used there is no means of knowing or of stating their physiological effectiveness in other than the most general terms. An induction shock is weak, medium, or strong. More closely than that the user does not attempt to describe it.

This lack of knowledge as to the strengths of the stimuli employed is often a serious handicap in the prosecution of individual researches, particularly such as call for the use of stimuli of varying strengths. It also operates to make uncertain the attempts of investigators to duplicate the experiments of others.

No one will question the desirability of being able to measure faradic stimuli, both for the sake of controlling the stimuli used in one's own experiments, and also in order that these stimuli may be so described as to enable other workers to duplicate them as occasion arises.

The purpose of this work is to outline a system for calibrating the apparatus used in generating induction shocks, so that the value of the shocks may be expressed in terms of stimulation units; these units to be applicable to any properly constructed induction apparatus, and to be based upon determinations which can be made in any ordinarily equipped physiological laboratory. The system proposed is not a new departure, but is an extension and amplification of previous systems.

Historical. The phenomenon of electromagnetic induction was discovered by Faraday in 1831, and its physical characteristics were very thoroughly worked out by him and by Henry about the same time. The first suggestion for the physiological use of induction shocks appears to have been made by Sturgeon* in 1837, and from that time to the present their use in this connection has continued.

Various forms of induction apparatus have been de* Annales de Sturgeon: 1837, p. 477.

vised, but for physiological purposes only one has come into common use; this form, designed by E. du Bois-Reymond* in 1848, is illustrated in Figs. 1 and 2. Such modifications of this design as have arisen since its introduction have to do only with details, and not at all with the underlying principle of the apparatus.

Structure of the Inductorium. The induction coil, as adapted by du Bois-Reymond to physiological use, con-

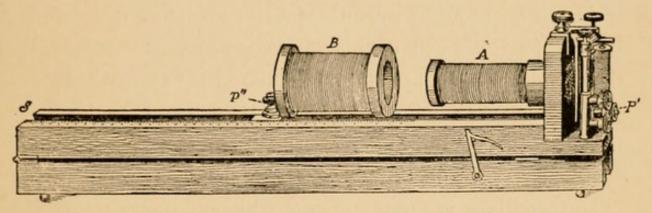


Fig. 1. The induction coil as used for physiological purposes (du Bois-Reymond pattern): A, the primary coil; B, the secondary coil; P', binding posts to which are attached the wires from the battery—they connect with the ends of coil A; P'', binding posts connecting with ends of coil B, through which the induction current is led off; S, the slide, with scale, in which coil B is moved to alter its distance from A.

sists, in essence, of two coils of carefully insulated copper wire. One of these, the *primary* coil, is made up of two or three layers of rather coarse wire wound upon a hollow core of nonconducting material. Usually the outside diameter of this coil is about 2.5 to 4 cm., and its length between 8 and 14 cm. The number of turns

* du Bois-Reymond: Unters. über tierische Electrizität, 1848, Bd. 1, S. 447; also, Bd. II, 1, S. 393.

of wire does not ordinarily exceed 600. The coil is mounted horizontally by one end upon a suitable support. The ends of the wire are brought to two binding posts, situated at some convenient place on the support.

The other coil, the secondary, consists of numerous turns of very fine insulated wire, wound upon a hollow spool whose inside diameter is such that the secondary coil can be brought over the primary. The number of turns of wire is usually between 5000 and 10,000. The length of the secondary coil is about equal to that of the primary. The ends of the wire are brought to binding posts mounted upon the spool. A slide, 30 or 40 cm. long, projects from the support of the primary. The secondary is mounted upon this slide with its axis coincident with the axis of the primary. A scale, graduated in millimeters, is mounted on the slide. A pointer on the secondary coil is so placed that it indicates zero on the scale when the secondary covers the primary completely. A device for making and breaking the primary circuit automatically is usually included as part of the apparatus; and a bundle of soft iron wire, so constructed as to slide into the hollow core of the primary coil, is likewise provided.

Principle of the Inductorium. Whenever a steady current is flowing through the primary coil there exists about it a magnetic "field of force." This field may be

pictured as consisting of "lines of force" each of which passes lengthwise through the primary coil, and, extending a greater or less distance from it into space at either end, curves outward and back so that the two ends meet, making each "line of force" a closed ellipse. The lines of force are very numerous near the primary coil, but become less and less frequent as the distance from the coil increases. The number of lines of force present and the distance from the coil at which they can be detected depend upon the intensity of the current flowing through the coil.

If another coil of wire, the secondary, be placed within the field of force about the primary in such position that lines of force pass lengthwise through it, any alteration in the number of lines of force comprehended within the secondary generates within it a current which is the induced current. This current, which depends upon changes within the field of force, ceases to be generated whenever the field of force becomes steady, and outlasts the change in the field only the brief fraction of a second required for the current to die away. The direction of the induced current depends upon the direction of the current through the primary coil, and also upon whether the change in the field is an increase or a decrease in the number of lines of force. The intensity of the currents induced in any secondary coil depends upon the number of lines of force moving through it,

and also upon the *rate* of their movement; the more rapid the change in the field, the higher the intensity.

The method used in physiology for bringing about alterations of the field within the secondary coil is to make and break the current through the primary.

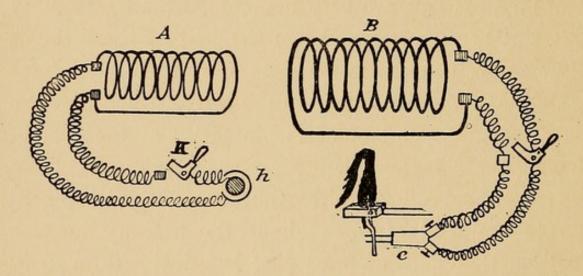


Fig. 2. Schema of induction apparatus (Lombard). h represents the galvanic battery connected by wires to the primary coil A. On the course of one of these wires is a key, k, to make and break the current. B shows the principle of the secondary coil and the connection of its two ends with the nerve of a nerve-muscle preparation. When the battery current is closed or made in A, a brief current of high intensity is induced in B. This is known as the making or closing shock. When the battery current is broken in A, a second brief induction current is aroused in B. This is known as the breaking or opening shock.

When the primary current is made there is a sudden increase in the lines of force cutting the secondary coil; when the primary current is broken these lines of force suddenly disappear. The currents induced by the make and the break of the primary circuit are obviously of

very short duration, since the time required to establish the field of force on the one hand, and for its disappearance on the other, is measured in thousandths of a second, and, as we have seen, only during these periods do induced currents flow. The current induced in the secondary by the *make* of the primary circuit is usually spoken of in physiology as the make shock; that induced by the *break* of the primary is the break shock.

A feature of induction shocks which commends them particularly to the physiologist is the ease with which their intensity may be varied. For securing this variation advantage is taken of the dependence of the induced current upon the number of lines of force which cut the secondary coil. There are two ways of varying this number: One is by changing the intensity of the primary current; the other, by shifting the position of the secondary coil with reference to the primary. This latter method is the one used in the du Bois-Reymond inductorium, and it is a very satisfactory method, since by means of it the strength of the stimulus can be varied several hundredfold, from the maximum for the apparatus to a value negligibly small, by simple shifting of the secondary from one end of its slide to the other. Many inductoria are so constructed that the secondary coil can be rotated about an axis midway of its length. In this way the intensity of the induced current can be cut down to zero, since when the secondary is at right angles to the primary no lines of force pass lengthwise through it. For quantitative purposes, however, it is better to have a rather long slide and to keep the secondary coil always with its axis coincident with that of the primary.

The Form of Make and Break Induced Currents. When a circuit is closed through the primary coil of an inductorium there is a growth of the current within this coil from zero to its full value. Coincidently with this growth of current there is being established a field of force about the coil, and if there is a secondary coil within this field a current is being induced therein. This induced current also begins at zero and increases in intensity during the establishment of the field of force about the primary. As soon as the field is fully established, so that movement of the lines of force ceases, there is no further induction and the current within the secondary dies away. We may represent the successive changes in intensity of the induced current by a curve such as that shown in Fig. 3 in which the height of the curve at any point represents the intensity of the induced current at that instant.

The rise of the make induced current from zero to the maximum, although rapid, is by no means instantaneous, there being a well marked delay in the establishment of the current through the primary coil after the circuit is closed. This delay is due to the phenomenon of *induc*-

tance within the primary coil. This phenomenon may be explained as follows: When the current sweeps through any turn of wire of the primary coil it tends to establish a field of force about that turn; but as the lines of force composing this field cut through adjacent turns of wire of the primary they induce currents therein. Since energy is expended in this inductance the currents thus induced cannot be in the same direction as the inducing current; inasmuch as if they were, there would be a

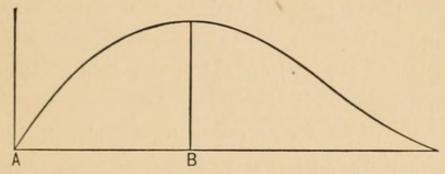


Fig. 3. Curve illustrating the growth and decline of a make induced current. AB represents the time required for the primary current to become fully established.

gain of energy — a thing impossible; they oppose the inducing current and allow it to reach its full value only after it has yielded the energy necessary for the inductance. In Fig. 3 the line AB represents the time occupied by the primary current in establishing itself against the inductance, and therefore the time during which the induced current increases.

Any condition which diminishes the inductance within the primary coil, thereby allowing the primary current to establish itself more quickly, will not only make the ascending limb of the curve of Fig. 3 steeper, but will also carry it higher; that is, the current induced in the secondary will not only reach its maximum intensity more quickly, but that maximum will be greater; this result being due to the fact that the intensity is greater the more rapid is the alteration in the field of force cutting the coil.

While a current is flowing steadily through the primary coil no induction is manifest; but when the current is broken there is produced in the secondary coil a break induced current. The agency generating this current is the sudden withdrawal of the field of force from the secondary coil.

With the breaking of the primary circuit it would seem at first thought that the lines of force should disappear instantly and that there should be an instantaneous leap of the break induced current from zero to maximum. As a matter of fact the growth of the break current, although very rapid, is not instantaneous, for the reason that with the breaking of the primary circuit the energy absorbed from the current at its make by the inductance within the coil is released and manifests itself as the "extra current," jumping across the points of broken contact as a spark and prolonging slightly the decay of the primary current.

The chief difference between Fig. 10, p. 33, which represents the course of a break induced current, and Fig. 3,

representing a make current, lies in the greater steepness of the ascending limb of the curve of the break current, due to the shorter period occupied by the spark in passing. Here again any condition that hastens the passage of the spark brings about increased intensity of induced current by accelerating the disappearance of the field of force.

Since under most conditions the delay in establishing the primary current, due to inductance, is greater than the delay in its disappearance, from sparking at the contacts, make shocks are usually less intense physiologically than are break shocks.

CHAPTER II

FACTORS WHICH AFFECT THE STRENGTHS OF FARADIC STIMULI

Any scheme for measuring induction shocks, if it is to be wholly satisfactory, must take into account all the sources of possible variation present in the mechanisms by which the shocks are generated and applied to tissues. The numerous methods which have been worked out hitherto have been uniformly based upon sound physical principles, and give accurate results so far as they go; they leave something to be desired, however, in that none of them deals with all the conditions of variation which are actually present whenever tissues are stimulated, and their usefulness is limited by just that much. The justification for the present work lies in its attempt to take into account all the sources of variation which exist. These are to be divided into those whose influence upon the strength of stimuli is in accordance with mathematical laws, determinable by the experimenter, and those which are not apparently so determinable. The former are made the basis for the system of measuring stimuli herein described; the latter are studied with a view to showing how their effects may be minimized.

Sources of Variation. The induction apparatus, as used in the physiological laboratory, consists of two circuits: the primary, or inducing circuit, which includes the primary coil of the inductorium, a source of current, and a device for making and breaking the circuit, together with the necessary connecting wires; and the secondary circuit, including the secondary coil, wires leading thence to suitable stimulating electrodes, and the tissue to be stimulated. In Fig. 2, p. 6, these circuits are illustrated diagrammatically.

In any given primary circuit variations may arise either in the amount of current yielded by whatever source of current is used; or in the key, whereby the circuit is made and broken. In any given secondary circuit variations may arise in the position of the secondary coil with respect to the primary, this being, as we have seen, the usual method of bringing about variations in stimulating strength; in the electrical resistance of the tissue which is being stimulated; and in the contacts between the stimulating electrodes and the tissue to which they are applied. Also different inductoria usually present structural differences, such as different dimensions and different numbers of turns of wire in primary and secondary coils, which themselves bring about wide differences in the strengths of stimuli generated by the different inductoria. The presence or absence of an iron core within the primary coil is also

a source of great modification of stimuli. Finally, as we have seen, there is a difference in physiological effect between make shocks and break shocks.

Of the sources of variation just described the following are subject to laws which are determinable, and are to be included, therefore, in our quantitative scheme: The construction of the inductorium, the position of the secondary coil with respect to the primary, the presence or absence of an iron core in the primary, the intensity and voltage of the primary current, the use of make or break shocks, the electrical resistance of the stimulated tissue and the mode of contact of the stimulating electrodes with the tissue.

The variable which is not determinable is the effect on the stimulus of the manner of making or breaking the primary circuit. This must be, so far as possible, made uniform.

Methods Previously Proposed. The first attempt to measure induction shocks is said to have been made by Rosenthal in 1857.* Two years later Pflüger made quantitative comparisons between shocks, varying their intensities by varying the primary current, leaving all other factors constant. His method gives accurate relative results, but seems not to have commended itself to physiologists, probably because it calls for a rather com-

^{*} See Garten: Handbuch der physiol. Methodik, 1908, Bd. II, Abt. 3, S. 393.

plex mechanism for varying and at the same time measuring the primary current.

The earliest method of measuring induction shocks which received wide recognition was worked out under the direction of Fick by his student, Meyer, in 1869.* This method concerned itself altogether with the effect upon the intensity of break shocks of shifting the position of the secondary coil relative to the primary, and amounts, therefore, to a calibration of the slide upon which the secondary coil moves. By such calibration the relative intensities of the shocks given by the inductorium at the various secondary positions are accurately indicated, so long as all the other variable factors remain unchanged. A similar calibration is an essential feature of any scheme for the quantitative use of the inductorium, and indeed the only criticism of the Fick method of measuring stimuli is for its incompleteness. The Fick calibration was accomplished by including in the secondary circuit a galvanometer and determining the current induced in the secondary coil at its various positions by the deflection produced when a given current was made or broken through the primary. This method, although simple in theory, was in fact rather difficult to put into practice with the electrical measuring apparatus available in Fick's time; and accordingly

^{*} Meyer: Unters. phys. Labor. d. Züricher Hochschule, Wien, 1869, S. 36.

Kronecker,* in 1871, introduced a modification of the method whereby its application was simplified. He used two inductoria, connected their secondary coils in series with a galvanometer and connected both primary coils with a single source of current in such fashion that the two secondaries gave induced currents opposite in direction when the primary circuit was broken. Thus the galvanometer deflection was used merely as an indicator that one induced current was stronger than the other, rather than as a measure of the strength of the induced current itself.

With both secondaries at zero the primary current was broken and the amount and direction of deflection noted. The coil giving a stronger shock was then moved outward till no deflection occurred. Then the weaker coil was moved outward till a deflection equal to the first one was obtained. This procedure was repeated till the whole length of the slide had been traversed, the number of times the stronger secondary was moved being noted. If this number is multiplied by the original galvanometer deflection we have a value which expresses how many times greater the galvanometer deflection would be with the secondary at zero than at the end of the slide. To calibrate the slide on the basis of 1000 units, as Kronecker does, the total deflection noted

^{*} Kronecker: Arbeiten aus der physiologischen Anstalt zu Leipzig, 1871, S. 186.

above is divided by 1000 and the quotient gives the galvanometer deflection per unit. If now the weaker coil is set at zero and the stronger at a point such that the galvanometer deflection is that called for per unit, it is possible, by repeating the original procedure, to divide the scale into 1000 parts, each of which represents a given galvanometer deflection, and therefore an equal decrement in stimulating value. This method has the advantage that after one inductorium is calibrated it is extremely easy to calibrate others to correspond with it, by connecting the calibrated and uncalibrated coils in the manner described above and finding the corresponding points on the two slides. Kronecker, by substituting a telephone for the galvanometer, made the taking of readings even more simple.

The method has the disadvantage that it is purely arbitrary, depending at the outset on a chance difference of stimulating strength occurring in two inductoria; for this reason the calibration can only be duplicated through access to a coil already calibrated. An observer, unable for any reason to obtain a Kronecker coil, might, it is true, prepare a calibration of his own by repeating Kronecker's original procedure, but he could not know whether his units represented the same stimulating values as the corresponding Kronecker units, and so could not express satisfactorily the strengths of stimuli used by him.

v. Fleischl,* in 1875, proposed a method of calibrating the inductorium in which for the galvanometer deflection was substituted the threshold contraction of a nerve-muscle preparation. In this calibration the decreases in stimulating value which result from moving the secondary coil outward were compensated by increasing the current through the primary coil, the increases required being taken as the measure of the change in stimulating intensity resulting from the movement of the secondary. This method has the advantage of being available in situations where no galvanometer can be obtained. Its greatest importance lies, however, in confirming the assumption of Fick and of Kronecker that the physiological intensities of break induced currents are proportional to the galvanometer deflections they produce.

Wertheim-Salomonson† has recently described a method for obtaining a physiological calibration in which variations in the primary current are avoided. He places the nerve of the nerve-muscle preparation to be used as an indicator in one branch of a divided secondary circuit, and in the other branch places a resistance equal to that of the nerve. (See Fig. 4.) The resistance of the divided circuit is then one-half that of

^{*} v. Fleischl: Sitzb. d. k. Akad. d. Wissensch. Wien, 1875, Bd. lxxii, Abth. III. Also Ges. Abh., 1893, S. 475.

[†] Wertheim-Salomonson: Zeitschr. f. Elektrother. I., 1899, S. 97.

the nerve alone. By placing in the circuit beyond the shunt another resistance equal to one-half that of the nerve the total resistance of the secondary circuit is made equal to what it would be if the shunt and the added resistance were both removed. Since, however, the nerve is in a divided circuit, both branches of which have equal resistance, it receives only one-half the current generated in the secondary coil. That secondary position at which the nerve receives threshold stimulation when in the divided circuit is determined, and then

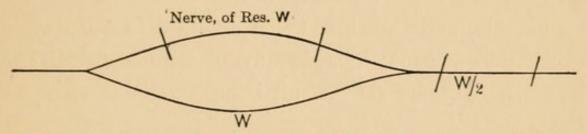


Fig. 4. Diagram showing method of inserting resistances in the Wertheim-Salomonson method of calibration. After Gasten.

Now the nerve receives the whole current from the secondary instead of half of it, and if the secondary position is found at which the threshold stimulus is again imparted we know that this second current has just half the stimulating value of the first. We have thus a method for comparing stimuli, which admits of extension sufficient for the complete calibration of a coil. It has, however, the shortcoming, already noted for Kronecker's method, of giving values applicable only

to the single coil on which it is worked out. One very important feature of a wholly satisfactory calibration must be its general applicability, so that any properly constructed inductorium can be calibrated in any laboratory to give results comparable with those obtained from other calibrated instruments.

Moreover, it is not to be forgotten that no method of calibration thus far described takes into account the effects of strength of primary current, of tissue resistance, or the method of applying the stimulating electrodes, all of which are important, and at the same time determinable, and therefore to be included in a complete calibration scheme; nor do any of them consider the strength of make shocks, all being available only for breaks.

A device which is superior in certain respects to any thus far described for measuring stimuli is the "faradimeter" of Edelmann. In this apparatus a galvanometer in the secondary circuit registers the voltage of the induced current. The galvanometer readings give correct indications of the values of stimuli only when a current of definite, fixed amperage is broken in the primary circuit. It is necessary, therefore, to have a source of currents specially selected to give this amperage, and by means of an ammeter in the primary circuit to insure that it is maintained. The Edelmann method is an advance over others in that it takes

account of the factor of primary current strength and provides for its regulation. It does not, however, take account of the influence upon the strength of stimulus of variations in tissue resistance, since the quantity measured by the galvanometer, namely the voltage, is independent of the resistance. Nor does it consider the effect of the method of application of the stimulating electrodes. But so long as these two factors remain constant the Edelmann faradimeter gives accurate results for break shocks, and expresses them in terms such that the stimuli used by one worker can, save for the factors above mentioned, be duplicated by others.

The importance of taking secondary resistance into account was brought out by Hoorweg* in 1893. He demonstrated the effect of variations in resistance in modifying stimulation strengths, and emphasized the necessity of working out some method by which to ascertain this effect. At his suggestion Giltay† designed an electrodynamometer by which the variations in strength of stimulus due to varying secondary resistances can be read directly. This apparatus fulfils admirably the purpose for which it was designed. It is, however, of little practical use in physiology, since its readings, to be comparable, must be made with the

^{*} Hoorweg: Die medicinische Elektrotechnik und ihre physikalischen Grundlagen, Leipzig, 1893.

[†] Giltay: Annalen der Physik und Chemie, 1893, Bd. 50, S. 756.

same inductorium or with inductoria of precisely similar construction, and the position of the secondary coil with respect to the primary must not be altered. In view of the fact that moving the secondary coil is the usual method among physiologists for varying the strength of stimulus, this instrument clearly does not altogether meet the requirements of physiological work. It has, moreover, the somewhat serious shortcoming of taking no account of the method of applying the stimulating electrodes, so that, even were all the other conditions met, the electrodynamometer would still fail to give wholly complete measurements.

Our examination of the various systems hitherto proposed for measuring induction shocks bears out the statement made at the outset that none of them meets fully the requirements of quantitative work. We are justified therefore in submitting a system which, although not new, being an extension of the Fick-Kronecker method, attempts to deal with all the factors concerned in the production of faradic stimuli, so that henceforth the values of stimuli may be expressed in such terms that they can be duplicated or modified quantitatively at will.

CHAPTER III

A SUMMARY OF PROCEDURE

For the convenience of users of the method herein presented it has been thought worth while to describe briefly at the outset the various pieces of apparatus used and to summarize the various procedures involved in making the necessary calibrations and in using the calibrated apparatus.

Instruments Required for the Calibration. The inductorium to be calibrated should be of "standard" construction (see p. 88), that is, it should have a secondary coil approximately 13 cm. long and having about 10,000 turns of wire. The number of turns and the mean cross section of the secondary coil must be accurately known (p. 55). The slide upon which the secondary moves should be not less than 30 cm. long. It should be accurately graduated in millimeters, and a pointer fixed to the secondary coil in such position as to stand at zero when the secondary is pushed completely over the primary. To increase the stimulating effectiveness of the instrument the primary coil should have a core made of a bundle of soft iron wires.

In addition to this inductorium there is needed a con-

stant source of current sufficient in amount to yield at least 1 ampere through the resistance of the primary coil. Where a charging current is available, probably a good storage battery will be found most convenient as a source of current. Several Daniell cells in series, how-

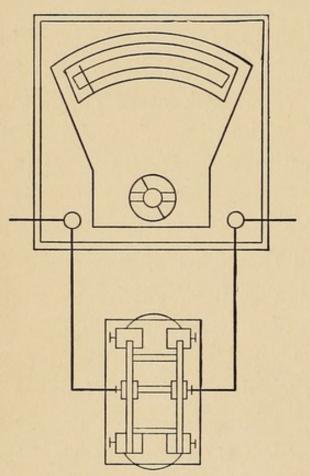


Fig. 5. Diagram showing ammeter the small currents with shunt made from a Porter metal-contact rocking key.

ever, answer every purpose. A good ammeter for measuring the intensity of the primary current is required, as is also a variable resistance for adjusting its amount. Since it is often necessary in the course of the work to use currents ranging from 0.0001 ampere to 1 ampere the ammeter must be able to cover this range. No instrument is, of course, able to measure sufficient accuracy and at the same time to give

direct readings for the larger ones. To give the ammeter the desired range, therefore, recourse must be had to a system of shunts. I have found it convenient to use a milammeter having a scale capacity of 10 mil am-

peres and reading directly to o.1 mil ampere, and to provide it with two shunts, one adjusted to carry ninetenths of the total current, the other to carry ninetynine one-hundredths of the current. For these shunts I use an ordinary Porter metal-contact rocking key connected as shown in the diagram, Fig. 5. For the 9 shunt, German silver wire is used between one pair of end contacts; for the $\frac{99}{100}$ shunt, copper wire is used between the other pair of end contacts. To calibrate the shunts, resistance is introduced into the ammeter circuit until exactly o.or ampere is flowing; then the shunts are adjusted until the ammeter reading is exactly 0.001 ampere, when the $\frac{9}{10}$ shunt is in circuit, and 0.0001 ampere when the $\frac{99}{100}$ shunt is in. The shunts must be recalibrated at frequent intervals, but this is not a difficult task.

As a means of adjusting the amount of primary current flowing I have found a dial resistance box most satisfactory, although any available variable resistance can be used. The total resistance should not be less than 11,000 or 12,000 ohms, since with a source of current yielding 2 volts that amount of resistance is often necessary to cut the current down to the point where threshold stimuli are produced.

For making and breaking the primary circuit some form of automatic key is required. A satisfactory one is described in Chapter IX. Experience shows that trustworthy results cannot be obtained with a key which fails to give uniform breaks. Uniform makes are very desirable, but for many sorts of work, including the routine of making the calibration, make shocks need not be employed.

All the apparatus thus far described is required for the quantitative use of the induction coil as well as for its calibration. Additional instruments needed for making the calibration are a good ballistic galvanometer and a standard induction apparatus. A satisfactory form of ballistic galvanometer is the d'Arsonval wall instrument with moving coil and reflected scale, read with a telescope. The standard induction apparatus can be made in any machine shop. It consists of a primary coil, at least 75 cm. long and composed of a single layer of heavy insulated wire, carefully wound, and a secondary coil, not over 15 cm. long, of about 2000 turns of fine wire, placed exactly at the center of the primary coil. The cross section and number of turns per centimeter of the primary coil must be known, and the total number of turns of the secondary.

Additional apparatus required in the use of the inductorium, but not in the calibration, is, first, a device for determining tissue resistance, and, second, suitable stimulating electrodes. I have found the Kohlrausch method of measuring resistance perfectly satisfactory (see p. 72). This method requires an ordinary meter

bridge, a small inductorium to give an alternating current, a telephone receiver for an indicator and a resistance box. By suitable wiring, illustrated in Fig. 15, p. 73, a single resistance box can be used both for varying the primary current and as the known resistance in the Kohlrausch determinations.

The stimulating electrodes must be selected with special reference to uniformity of contact. Accurate quantitative results cannot be gotten under conditions of contact variation. For the direct stimulation of muscles I have found platinum needle electrodes most satisfactory. A piece of platinum wire 2.5 to 3 cm. long, and 0.5 mm. in diameter, pointed somewhat at the end with a file, is soldered to a suitable length of very fine copper wire (diameter 0.2 mm.). The platinum needle is thrust directly into or through the muscle tissue; the copper wire, carried to the secondary terminal, affords the very flexible connection necessary for avoiding interference with the free movement of the muscle.

For stimulating nerves the glass-inclosed electrodes described by Sherrington * are as reliable as any I know of. They answer well either for the stimulation of nerves deeply imbedded within the body, or for stimulating the nerve of the ordinary nerve-muscle preparation. In the use of this form of electrode care must be taken that the

^{*} Sherrington: Jour. of Physiol., 1909, xxxviii, p. 382.

interior of the glass tube is clear of liquid. The electrode is shown in Fig. 6; contact is made by rotating slightly the stopper carrying the two platinum wires.

For the determination of "specific" stimulation values (see p. 76), a rather large known resistance, ten thousand to twenty thousand ohms, must be arranged to be included in the secondary circuit as required.

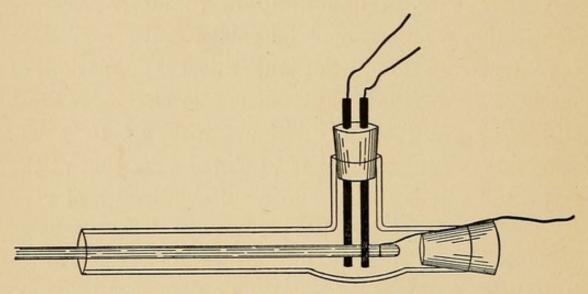


Fig. 6. Shielded electrodes (Sherrington).

The arrangement of apparatus for making the calibration is illustrated diagrammatically in Fig. 7. The procedure is by the following steps, for each of which a page reference is given.

- 1. Determination of the formula for core magnetization (p. 43).
- 2. Determination of the mutual induction for a series of selected secondary positions from 12 cm. outward (p. 38).

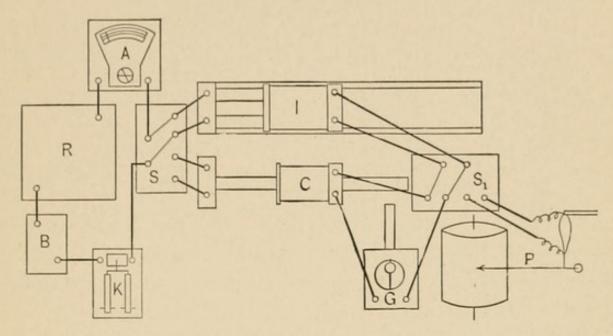


Fig. 7. Arrangement of apparatus for calibrating the inductorium. A, ammeter; B, battery; C, standard coil; G, galvanometer; I, inductorium to be calibrated; K, make and break key; P, apparatus for physiological calibration; R, resistance box; S and S_1 , switches.

- 3. Determination of the inductance of the secondary coil (p. 50).
- 4. Determination of $\frac{M}{L}$ for the secondary positions whose mutual inductions have been established (p. 53).
- 5. Physiological corroboration of this calibration by the v. Fleischl method (p. 56), accompanied by physiological determination of the "calibration numbers" for the inner secondary positions (p. 58).
- 6. Construction of a curve to establish calibration numbers for intermediate secondary positions (p. 56).
- 7. Determination of the constant C in the formula for make shocks (pp. 94 and 104).

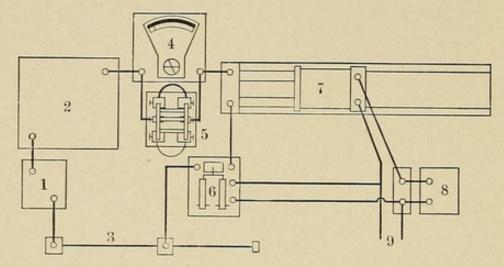


Fig. 8. Arrangement of apparatus for the use of the quantitative method. 1, battery; 2, resistance box in primary circuit; 3, slide wire resistance for fine adjustment; 4, ammeter; 5, ammeter shunt; 6, make and break key with automatic short-circuiting device for make or break shocks; 7, inductorium; 8, resistance box in secondary circuit; 9, wires leading to stimulating electrodes.

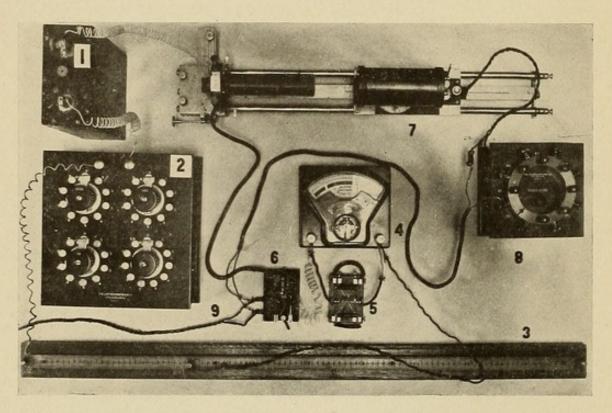


Fig. 9. View of apparatus in actual use. Significance of numbers is the same as in Fig. 8.

The arrangement of apparatus for the use of the quantitative method is indicated diagrammatically in Fig. 8. The diagram is self-explanatory. As an additional guide, a photograph of a set of apparatus in actual use is reproduced in Fig. 9. In the final chapter of the book various precautions are described which much experience with the method has suggested.

CHAPTER IV

THE PHYSICAL PRINCIPLES UNDERLYING THE MEASURE-MENT OF BREAK SHOCKS

Helmholtz* appears to have been the first to study in detail break induction shocks. He established the principles which are still accepted as to their formation and course. His work was chiefly from the physical standpoint, although he gave attention also to the physical ological aspect of the problem. More recently Fleming † has given a clear and concise discussion of break induction shocks, his presentation agreeing in every essential particular with the earlier one of Helmholtz. The following statement is, in the main, condensed from Fleming's discussion.

The Course of Break Induced Currents. The current induced in a secondary coil by the breaking of the primary current may be represented graphically by such a curve as is given in Fig. 10, beginning at zero, increasing rapidly to a maximum, and then falling more slowly away to zero. If the break of the primary were abso-

^{*} Helmholtz: Poggendorf's Annalen der Physik und Chemie, 1851, lxxxiii, S. 536. Also, Ges. Abh., S. 459.

[†] Fleming: The Alternate Current Transformer, London, 1892, i, pp. 184 et seq.

lutely instantaneous, the initial rise would be instantaneous likewise and the secondary current would begin with its maximum value. Since, however, there is always, even under most favorable conditions, a certain

amount of sparking at the contacts, there is never an instantaneous break, and the initial rise is constantly present. Helmholtz* demonstrated, with the aid of an ingenious apparatus, that the phys-

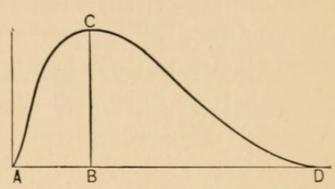


Fig. 10. Curve illustrating the course of a break induced current — after Fleming.

iological effect of a break induced current is chiefly exerted by that part embraced within the ascending limb of the curve. By breaking the secondary current at various points in its course he found that the physiological effect was virtually as great when the current was broken at the moment of reaching its maximum intensity as when it was allowed to run its entire course. Recent investigations carried out by means of short galvanic currents have shown, it is true, that the stimulating effectiveness of a shock is to some extent dependent as well upon the descending portion of the curve,† so that

^{*} Helmholtz: Loc. cit., S. 537.

[†] Gildemeister: Pflüger's Archiv für die gesammte Physiologie, cxxxi, 1910, S. 199.

Helmholtz' conclusion is not wholly valid. But at this stage of the discussion we may neglect the effect of the descending portion of the curve, and proceed as though the ascending limb were the sole determining factor.

Since the chief physiological effect is exerted during the growth of the current this effect will be greater the higher the curve rises; in other words, the strength of stimulus tends to be proportional to the maximum intensity of the induced current. In the diagram, Fig. 10, the maximum intensity is represented by the ordinate *CB*, drawn from the base line to the summit of the curve, and with the factors determining the value of this ordinate we are at present concerned.

Helmholtz showed that the induced current reaches its maximum intensity at the instant the spark ceases to pass. The abscissa AB, therefore, represents the time occupied by the spark. In a properly constructed apparatus AB will be constant. Helmholtz showed also that the value of the ordinate CB is approximately equal to $\frac{MI}{L}$, in which M is the mutual induction be-

tween primary and secondary, I the intensity of the current through the primary, and L the inductance of the secondary. If the break were instantaneous, making AB zero, CB would equal the expression given above; it falls below that value more and more as AB increases, but so long as AB is constant the relation between the

true value of CB and the value $\frac{MI}{L}$, which it approximates, does not vary.

We may use the expression $\frac{MI}{L}$, therefore, as a physical basis for the measurement of break shocks, although we must note that the expression will not serve fully, since the factor of secondary resistance is not included in it, nor is there any factor for the influence of the manner of applying the stimulating electrodes. Moreover, the expression is proportional to the strength of the stimulus only so long as the circuit is broken uniformly. The expression serves in our quantitative scheme, therefore, only as a starting point. Its use even so far is justifiable only if physiological tests confirm the applicability of the physical relationships. That they do so completely will be shown in due course.

Our next step is a consideration of the individual factors in the expression $\frac{MI}{L}$ and a discussion of the means whereby they are to be determined.

Of the three factors which make up the expression, one, I, the intensity of the primary current, is an easily measured electrical quantity, and is best determined directly by means of an ammeter in the primary circuit. The other two, M and L, are functions of the construction of the inductorium, either by itself or as modified

by the relative positions of the primary and secondary coils. M, the mutual induction between the primary and secondary coils, varies with changes in the position of the secondary relative to the primary, but is fixed for each position. It can therefore be determined once for each position of the secondary coil, and the values thus obtained used in all future calculations.

Since mutual induction is the factor which varies with shifts in the position of the secondary coil relative to the primary, most of the calibrations hitherto proposed amount in effect to determinations of the relative mutual inductions for the various secondary positions. That the stimulating power should theoretically be proportional to the mutual induction so long as the other factors remain constant is obvious from inspection of the

expression $\frac{MI}{L}$. That the proportion really does exist is proved by the experimental verification of the Fick,

Kronecker, and Edelmann calibrations, as well as by the experiments carried out in the development of the present method.*

L, the inductance of the secondary coil, is a function of the construction of the coil and is therefore constant for any given inductorium except as it is modified by extraneous influences. When the inductorium is used

^{*} Martin: Amer. Jour. of Physiol., 1908, xxii, p. 123.

with an iron core in the primary, this acts to modify the value of L whenever the secondary coil is directly over the iron core.

The methods by which M and L are determined in practice are outlined in succeeding chapters.

CHAPTER V

THE DETERMINATIONS OF MUTUAL INDUCTION BETWEEN PRIMARY AND SECONDARY COILS

In determining the mutual induction for the various secondary positions advantage is taken of the fact that this factor appears in the expression for the integral effect of the induced current. This integral effect is represented in the diagram (Fig. 10), by the entire area ABCD; its expression is $\frac{MI}{R}$, in which M and I have

the same meanings as hitherto, and R equals the resistance in the secondary circuit. The integral effect can be measured by means of the ballistic galvanometer. For this purpose the secondary of the induction coil under examination is connected in series with a good ballistic galvanometer and with the secondary of a standard induction coil, the latter apparatus being so constructed that the mutual induction between its primary and secondary coils can be computed from the construction of the apparatus and the current through the primary. The special features of its construction are found in the primary, which is a solenoid of one-layer thickness, very evenly wound, and several times longer

than the secondary. The lines of force through the secondary, placed at the middle of the primary, are then practically straight. The arrangement of the apparatus is shown diagrammatically in Fig. 7.

The secondary of the inductorium whose values of M are desired is set successively at points 1 or 2 cm. apart. At each point the galvanometer deflection caused by breaking a primary current of known intensity is determined. Since each galvanometer deflection represents a certain integral effect, no matter how produced, and since the integral effect affords means of computing M, a determination of the intensity of current which has to be broken in the primary of the standard coil to produce these same deflections provides all the data required for calculating the values sought. The formula used for computing M is developed in the following manner: The expression for the integral effect is, as stated above, $\frac{MI}{R}$. Let this represent the galvanometer deflection caused by breaking a current of intensity I in the primary of the coil whose values of Mare desired. Let the expression $\frac{M'S}{R}$ represent the same galvanometer deflection caused by breaking a current of intensity S through the primary of the standard coil. Equating these, we have $\frac{MI}{R} = \frac{M'S}{R}$. The method of

connecting the secondaries is, as stated previously, purposely such that the value of R is constant throughout. It therefore disappears from the equation and we have MI = M'S. The value of M' is computed from the construction of the standard coil according to the formula $M' = 4 \pi n NAS$, in which n equals the number of turns in the primary coil per centimeter of length, N the total number of turns in the secondary coil, A the area of the cross section of the primary, and S the current through the primary in electromagnetic units. Since this current is measured in amperes, it is necessary in practice to call S the intensity of the primary current in amperes and divide the expression by 10 to reduce to electromagnetic units. The formula for M' then becomes $\frac{4 \pi n NAS}{10}$. The value $\frac{4 \pi n NA}{10}$ is constant for any given standard coil, and once determined is substituted for M' in the equation MI = M'S.

To illustrate the process of determining mutual inductions by this method, suppose the standard coil has the following dimensions:

Number of turns in primary per centimeter... 5.4

Total number of turns in secondary...... 1865

Area of cross section of primary...... 6 sq. cm.

The value of $\frac{4 \pi n N A}{10}$ is 75,870, and the equation for mutual induction is $M = \frac{75,870 \, S}{I}$. Now suppose that

with the secondary coil at 12 cm. from the zero position the breaking of a primary current of 0.1 ampere gives a deflection on the galvanometer scale of 5, and that to secure the same deflection with the standard coil a current of 6.8 amperes must be broken through its primary. Substituting these values in the equation we obtain for M 5,150,000. By repeating this procedure the values of M for every secondary position can be obtained.

If $\frac{MI}{L}$ is a true expression for the physiological effect

of break shocks, evidently with L constant the product MI must also be constant so long as it represents a uniform stimulus, no matter how the value of M may be varied by shifting the secondary coil. Experiment shows that MI does remain constant for a constant stimulus over the entire field of the inductorium, except that, when an iron core is present, it varies in the part of the field directly over the iron core. This is the region in which, as stated in a former paragraph, the value of L is affected by the presence of such a core.*

If a constant stimulus gives a constant value of MI, however the secondary coil may be shifted, it follows that if I is made constant,—in other words, if a fixed current is broken through the primary coil,—the strengths of stimulus at different secondary positions must vary

^{*} For experimental evidence, see Martin: Amer. Jour. of Physiol., 1908, xxii, p. 124.

directly as the values of M for those positions. By determining these values, then, we provide ourselves with a calibration which reveals accurately the effect on stimulating strength of shifting the secondary coil. Such a calibration, as previously stated, is a necessary basis in any scheme for the quantitative use of induction shocks.

CHAPTER VI

EFFECTS PRODUCED BY AN IRON CORE IN THE PRIMARY COIL

INASMUCH as the almost universal practice in physiological work is to use inductoria with iron cores, a brief discussion of the effects of such cores on stimulation strengths seems desirable at this point. Thus the method becomes at once applicable to inductoria with iron cores as well as to those not provided with them.

The principal effect of the iron core is that which has led to its use, namely a great increase in the number of lines of force surrounding the primary coil, with a corresponding increase in the intensity of the stimuli generated.

Another effect is that noted in a previous paragraph (p. 36), of altering the effectiveness of the stimuli generated when the secondary coil is directly over the primary, so that in these positions MI is not constant for a constant stimulus. The method of correcting the calibration for this effect of the iron core is given in Chap. VIII, p. 58.

The iron core has also an effect upon stimulation strength due to its *magnetization* by the primary current, an effect which appears, however, only when primary currents of considerable intensity are used. Allowance

for this effect in computing the values of MI must be made, whenever I is large, by introducing a correction factor. This factor can be obtained without difficulty by the use of the ballistic galvanometer, since the deflections of that instrument are affected by core magnetization. Inspection of the formula MI = M'S (p. 40) shows that so long as M and M' remain constant, I, the current through the primary of the coil under examination, must vary directly as S, the current through the primary of the standard coil. This relationship is found by experiment to hold in ordinary induction coils for values of I up to 0.1 ampere, but above that point the value of S is always larger than the equation calls for. In other words, when core magnetization is present the primary current produces a greater deflection than it does in the absence of this effect. The variation due to the magnetization of the core is not very difficult to correct, because, as repeated experiment has shown, the ratio between the actual values of I and those computed from the values of S depend upon an easily determined factor which is constant for any given iron core.

To determine this factor some position of the secondary coil must be selected at which primary currents up to 1 ampere give galvanometer deflections not greater than the entire scale. With the secondary in this position primary currents of increasing intensity, beginning at about o.o1 ampere, are broken, and the deflections

produced by each carefully noted. Then with the standard inductorium the values of S giving these same deflections are determined. Although at first the ratio of S to I remains constant, as the values of I begin to exceed o.1 ampere the ratio steadily increases. It is evident, therefore, that large currents are producing relatively greater deflections than small ones. By multiplying the different values of S by the ratio of S to I, which was constant, we obtain a series of computed values of I representing the currents which would be required to produce the observed galvanometer deflections if no iron core were present. These are, of course, the values of I which are to be employed in computing the strengths of stimuli according to the expression $\frac{MI}{L}$.

Table I, column 3, gives the values of I computed from a series of observed values of I and S in actual experiments.

TABLE I

Value of I observed in amperes.	Value of S observed.	Value of I computed in amperes.	Ratio computed value of I to its observed value.	Decimal part of ratio divided by observed value of <i>I</i> .	
0.01	0.005	0.01	1.0		
0.05	0.025	0.05	1.0		
0.10	0.05	0.10	1.0		
0.20	0.1044	0.2088	1.044	.22	
0.30	0.1597	0.3194	1.065	.217	
0.40	0.2180	0.4360	1.000	. 225	
0.50	0.2782	0.5564	1.113	. 226	
0.60	0.3396	0.6792	1.132	.22	

To derive the equation for obtaining I computed when I observed is known we determine in a series of experiments the ratios of I computed to I observed (see column 4 of the table). If now the decimal part of each ratio is divided by its corresponding value of I observed, a constant is obtained which represents the number by which I observed must be multiplied to obtain this decimal part of the ratio. This constant is shown in column 5. After the constant is found it is used for computing I according to the formula $I_c = I_0 \times (I + KI_0)$. In this formula I_c is the computed value of I, I_0 is its observed value, and K is the constant, — in the case cited in the table equaling .22.

The method of correcting for the magnetization of the iron core is given in detail since, in spite of the abundant theoretical justification for the omission of the iron core, especially where quantitative estimations are sought, for the practical purposes of the physiologist the inductorium as commonly used, with the iron core present, is usually to be preferred. The intensity of stimulus, other factors being equal, is at least five times greater with the iron core than without it in inductoria of the usual type. This increased efficiency makes it possible to obtain with primary currents of moderate intensity as strong stimuli as the physiologist ordinarily requires. The use of *moderate* primary currents is of great importance in quantitative estimations of induc-

tion shocks, since thereby is avoided that heavy sparking at the contacts which always accompanies the break of a current of high intensity, and which affects the intensity of the stimulus in a manner that cannot be foretold.

When the secondary coil of an inductorium is moved from the zero position until nearly clear of the primary coil, it enters a "critical region" where small changes in position are accompanied by great changes in the intensity of the stimuli given by the instrument. The impression seems to prevail among physiologists that inductoria having iron cores show so much greater variations of intensity in this "critical region" than do those without iron cores as to make the omission of the iron core a distinct advantage in many experiments. As a matter of fact, however, Kronecker inductoria, such as are used in most physiological laboratories, show for given changes in secondary position in the "critical region" greater variations in stimulation intensity with cores removed than with cores present. This is apparent when the Kronecker graduations of such coils are compared with the calibrations made for them by the method of the present work (see p. 55). In the preparation of the Kronecker graduations the iron cores were withdrawn from the instruments. For the calibrations made in connection with this work the iron cores were in place.

TABLE II

Effect of the Iron Core on the Rate of Change of Stimulation
Intensity in the "Critical Region" of the Inductorium

Position of sec-	Iron co	ore absent.	Iron core present.		
ondary in cen- timeters.	Kronecker graduation. Percentage decrease per centimeter.		Author's calibration.	Percentage de- crease per centi- meter.	
8	6190		6240		
9	5150	17.0	5340	14.4	
10	4150	19.4	4500	15.7	
II	3250	21.7	3600	20	
12	2375	27.0	2640	26.7	
13	1570	33.9	1920	27.3	
14	1000	36.3	1270	33.8	
15	625 37.5		860	32.I	
16	435	30.4	600	30.3	
17	310	28.7	455	24.2	
18	230	25.7	350	23.I	
19	178	22.7	280	20.0	

Table II gives a comparison of the calibrations in the "critical region" of one inductorium made without and with the iron core. The primary coil of this instrument was 14 cm. long. The table shows clearly that the rate of decrease of stimulation intensity from point to point is greater when the iron core is absent than when it is present. Table III is the record of experimental verification of the same fact. Stimulation intensities were compared in these experiments according to the v. Fleischl method (p. 56), namely by comparing the primary currents required to produce stimuli of equal value with the secondary coil at different positions.

According to this method increases in the primary current represent corresponding decreases in the stimulating efficiency of the inductorium.

TABLE III

Experimental Proof that Stimulation Intensity shows Greater Variation in the "Critical Region" when the Iron Core is Absent than when it is Present. Break Shocks

		Iron core absent.		Iron core present.	
Date of experiment.	Position of secondary in centi- meters.	Primary current, amperes.	Per- centage increase in cur- rent.	Primary current, amperes.	Per- centage increase in cur- rent.
Dec. 21, 1906	8.0	0.0195	150	0.00187	148
	16.0	0.260	415	0.022	375
Dec. 24, 1906	8.0	0.00576		0.0008	
	12.0	0.01523	164	0.00197	146
	16.0	0.091	432	0.00934	374
Apr. 15, 1907	8.2	0.017		0.0036	
	11.28	0.035	107	0.0063	75
	12.45	0.0535	50	0.0092	46
	14.0	0.107	100	0.016	74
	16.2	0.2485	132	0.034	112

CHAPTER VII

COMPARISON OF ONE COIL WITH ANOTHER - THE VALUE OF L

WE have seen (p. 41) that in any given inductorium, after allowing for certain exceptions due to the iron core, if one is present, the strengths of stimuli produced by a given primary current with the secondary coil at various positions are directly proportional to the mutual inductions for those positions. When, however, the attempt is made to compare the stimuli generated by one inductorium with those produced by another, it is at once apparent that the relation between stimulating value and mutual induction holds only for stimuli produced by the same instrument. This, indeed, was recognized by Helmholtz, who pointed out the necessity of including in the expression for stimulating value the factor L, whereby to take account of the influence of inductorium construction. This factor, according to Helmholtz, is dependent on the inductance of the secondary coil, and is to be derived, therefore, from the expression for inductance. The common formula for

the inductance of a coil is $L = \frac{AW^2}{l}$, in which L is the

inductance of the coil, A its mean cross section, W the number of turns of wire composing it, and l its length.

When, in the course of developing this method of measuring stimuli, the attempt was made to apply the above expression for L in the formula $\frac{MI}{I}$, the curious observation resulted that it applied perfectly with some inductoria and not with others. That is to say, when equal stimuli were generated by means of different inductoria, equal values of $\frac{MI}{I}$ were given by some, but not by all, of the instruments compared. Upon analyzing the reason for the difference the following fact came out clearly; equal values of $\frac{MI}{I}$ were given by those inductoria whose secondary coils had the same number of turns of wire per centimeter of length, regardless of the total number of turns of wire; unequal values were given by those inductoria whose secondaries had different numbers of turns per centimeter of length. If we look now at the expression for L given above, i.e., $L = \frac{AW^2}{I}$, and separate within it the factor of turns per unit of length, the expression reads $L = AW \times \frac{W}{I}$. The experimental results showed as stated above that in all the inductoria

having the same value of $\frac{W}{l}$, namely the same number of turns per centimeter, the expression L = AW might be substituted for the expression $L = \frac{AW^2}{l}$ and equal values of $\frac{MI}{I}$ for equal stimuli would be given. next step was to see whether those inductoria which formerly gave non-concordant results would give concordant ones if for the value of L the expression AW, namely the product of the cross section of the secondary by the number of turns in it, were used. It was found that when this was done all the inductoria examined gave for equal stimuli corresponding values of $\frac{MI}{L}$, regardless of the dimensions of the coils, but subject to a certain restriction as to secondary resistance to be discussed later (p. 78). In order to bring this point out clearly some of the experiments upon which it is based are cited below (Table V). The inductoria used are described in Table IV. In this table only those inductoria are considered whose secondaries have different numbers of turns per centimeter, since only by them can be determined which of the two expressions for L is correct. In all the experiments, comparisons were made between the various inductoria and a single one known as coil B. This is a large inductorium with a Kronecker calibration whose secondary has 800 turns per centimeter; it was selected as a basis of comparison merely for convenience.

In Table IV, columns 5 and 6, are given, for the different inductoria examined, the values of L = AW and $L = \frac{AW^2}{l}$. To simplify the comparisons between the various coils the values of $\frac{AW^2}{l}$ as given in Table IV

were all divided by 800, the number of turns per centimeter in the secondary of coil B, thus making the value of L for coil B the same by either formula. These values are set down in column 7 of the table. To bring the final results into convenient denominations these figures and also those in column 5 were divided by 100. It is understood, of course, that these divisions, made purely for convenience, in no wise modify the relations between the coils.

In Table V are set down the experimental results of the comparisons between the various inductoria. Since details would only confuse, they are omitted. The figures presented in the table show clearly that the proper

expression for L is AW rather than $\frac{AW^2}{l}$.

Coil.	Length of sec- ondary coil.	Turns in secondary coil.	Cross section of secondary coil.	Cross sec- tion × turns in secon- dary coil.	Cross section × turns in sec.² length	Column 6 divided by 800.
B C F H N	cm. 13 7.4 13.5 9.3 9.3	10,350 4,830 3,000 6,000 8,000	sq. cm. 17.6 22 15.4 16.6 17.8	182,000 105,000 46,000 100,000 142,000	145,000,000 69,500,000 10,250,000 64,300,000 122,500,000	182,000 87,000 12,800 80,000 153,000

TABLE V Demonstrating that the expression for L should be AW rather than $\frac{AW^2}{l}$

$\frac{MI}{L}$ coil B .	Coil.	$\frac{MI}{AW}$.	$\frac{MI}{AW^2}$ $l \times 800$	$\begin{array}{c c} \underline{MI} \\ \overline{L} \\ \text{coil } B. \end{array}$	Coil.	$\frac{MI}{AW}$.	$\frac{MI}{AW^2}$ $l \times 800$
8 12.6 11.4 28.2 17 2.6 30.5 64	C F H	7.7 13 11.7 28 16.4 2.8 30.9 61.1	4.5 7.6 6.9 100 57 3.5 38.6 76.4	7.5 7 5.3 2.57 30.5 64 10.2 7.5	H	7·5 7·2 5·3 2·43 28.6 60 10.4 7	9.4 9 6.6 2.25 26.5 56 9.7 6.5

CHAPTER VIII

THE PREPARATION OF A CALIBRATION SCALE FOR BREAK SHOCKS

In previous chapters the methods of obtaining the individual factors making up the expression for break stimulation strength have been discussed in detail. To show how these methods are put into practice in preparing an inductorium for quantitative use is next in order. The first step is the determination of the mutual inductions by the method hitherto described, for a series of positions, preferably not more than 2 cm. apart, along the scale. If the instrument to be calibrated is without the iron core these measurements should be taken from the zero position outward; if an iron core is present there is no advantage gained by determinations of mutual induction for secondary positions in the region where the secondary coil overlaps the primary. Having determined these values, each is divided by L, the product of the cross section by the number of turns of the secondary coil. The mean cross section must be determined with great care, a rather difficult procedure in completed inductoria, and one which ought to be carried out in connection with their manufacture.

In order that the final stimulation units may be of convenient size the value of L which has been adopted in this scheme is not the direct product of the cross section by the number of turns of the secondary, but is that product divided by 100. Having determined this value, the mutual inductions previously established are divided by it. The resulting figures are the "calibration numbers" for the particular secondary positions to which they apply. To determine the numbers for intermediate positions those determined as above are plotted on a rather large scale on coördinate paper and a smooth curve is drawn connecting them. Since the mutual induction necessarily diminishes, not by fits and starts, but smoothly, as the secondary is moved outward, such a curve, if carefully made, will indicate the calibration numbers for intermediate positions with a high degree of accuracy.

To prove the accuracy of the calibration the method of v. Fleischl is employed (p. 18) in which the minimal contraction of a frog's gastrocnemius is used as the index of a constant stimulus. In detail this procedure as carried out by myself was as follows: The freshly isolated gastrocnemius was suspended by its attached femur in a moist chamber, and its lower end connected by a small copper wire to a muscle lever whose effective weight was about 10 gm.; the muscle was not afterloaded. The lever had a magnification of about ten, and its point pressed

lightly upon a smoked drum. The minimal contraction could be detected without difficulty, since the whole apparatus was made rigid enough for the slightest movement of the muscle to show itself at the end of the lever. Connection between the muscle and the terminals of the secondary coil was by means of two platinum needles soldered to fine copper wires leading from the secondary terminals. These needles were thrust directly through the muscle tissue, — one about 5 mm. below its origin, the other the same distance above the distal tendon, both in the same vertical plane. By this method of connecting the muscle, variations in the secondary resistance aside from those in the tissue itself were avoided. At least half an hour was allowed to elapse after the muscle was hung in position before stimulation was begun; in order that summation might not enter, the shortest interval allowed between successive stimuli was ten seconds; to avoid fatigue the strength of stimulus used was always kept as near minimal as possible. The results of repeated experiments show that under these conditions a high degree of constancy is usually maintained during the interval, about three hours, required for a single experiment. That each experiment be complete in itself is, of course, necessary, since no means has suggested itself for obtaining a response which shall remain constant through a period of successive days. To have conditions uniform the electrode nearer to the

origin of the muscle was in most cases made the cathode. With the minimal contraction of the muscle as the index, the primary current necessary to arouse it, measured in amperes, is determined with the secondary coil in various positions. To allow for variations in irritability of the tissue the experiment should be repeated a number of times. If the calibration is carefully made in the beginning it will be found that in each individual experiment the product $\frac{M}{L} \times I$,—primary current times calibration number,—is virtually constant, showing that the calibration is correct.

Should the inductorium being calibrated have an iron core, there still remains the establishment of calibration numbers for the region where the secondary coil overlaps the primary. These, however, can easily be determined by extending the experiments, just described for proving the calibration, to cover this part of the field. The value of $\frac{M}{L} \times I$ is established in any

given experiment from the part of the field where $\frac{M}{L}$ is known, that is, where the calibration has already been worked out. Since this is constant so long as the stimulus is unchanged a determination of the primary current,

I, for this stimulus, in the region where $\frac{M}{L}$ is unknown,

yields at once data for computing $\frac{M}{L}$. By averaging several experiments this part of the field can be calibrated with sufficient accuracy.

It must be stated, however, that in the innermost part of the field, including about half of the length of the primary coil from zero outward, the calibration numbers determined by the v. Fleischl method will be found to differ somewhat according as the tissue used as an indicator has high or low resistance, high resistances showing larger calibration numbers than low ones. For this reason it is desirable to avoid using this region in work which requires a high degree of accuracy, unless a calibration has been previously worked out for the resistance actually to be employed. Experience shows that occasions when it is necessary to use the first 5 or 6 centimeters of the scale are of rare occurrence in most kinds of experimental work.

CHAPTER IX

THE MAKE AND BREAK OF THE PRIMARY CIRCUIT

From the beginning of the use of induction shocks for stimulating living tissues investigators have recognized that the physiological intensities of these shocks are markedly affected by the manner of making or breaking the primary circuit. Helmholtz* called attention to this fact in his study of induced currents, and in the discussion of the variable factors to be considered in the attempt to measure induction shocks (p. 14), I pointed out that the manipulation of the primary key is a variable whose influence cannot be mathematically determined, and which, therefore, must be made as uniform as possible.

Before entering upon a discussion of means whereby the manipulation of the primary make and break key can be made uniform, it is desirable to point out briefly the manner in which variations in the break and make of the primary circuit modify stimulating intensities.

In the account of the theoretical basis for the break shock formula, $Z = \frac{M}{L} I$ (p. 34), the statement was

^{*} Helmholtz: Poggendorf's Annalen der Physik und Chemie, 1851, lxxxiii, p. 538.

made that this expression applies exactly only when the break is instantaneous, although it holds relatively so long as the time occupied by the break does not vary. Since this in turn depends on the duration of the spark, our present inquiry resolves itself, so far as break shocks are concerned, into a study of the conditions governing contact sparking.

The duration of the spark at a broken primary contact depends in part upon the intensity of the primary current, in part upon the amount of volatilization occurring at the contact, and in part upon the speed with which the points are separated. This last factor explains why keys operated by hand cannot be depended upon to give uniform results, and why some form of automatic key is required, since only thus can a uniform speed of separation be secured. Moreover, ordinary mercury keys cannot be depended on even when operated automatically, because of the tendency of mercury when not absolutely clean to cling in drops and thus vary the speed with which the contact points actually separate. In practically all keys there is some volatilization; platinum contacts giving the least, ordinary mercury contacts the most. It is impracticable to use always primary currents of a single intensity; but, in primary currents not exceeding 1 ampere, the variation is too slight to be of practical importance.

The making of a primary circuit is not attended with

sparking, so that the sources of error for makes are not the same as for breaks. As a circuit is made the resistance falls from infinity to the resistance of the closed circuit itself. It is during the change from the first of these resistances to the second that the secondary current is induced. The more nearly instantaneous the change, the greater is the physiological intensity of the induced current. In hand-operated metal-contact keys there can be no assurance that the contact points will be pressed together with the same firmness twice in succession, so that to secure uniformity of contact automatic keys are required for make shocks as well as for breaks. A further and more serious defect in metal-contact keys for make shocks is their liability to rebound slightly, or to slip sidewise, thus giving not a single clean-cut make, but a succession of make, break, and make. So constantly has this defect shown itself in my experiments, even with carefully constructed automatic metal-contact keys, that I have found it necessary to use mercury contacts altogether in studying make shocks.

The considerations stated above lead to the following conclusions: That hand-operated keys are not to be depended on for uniform makes and breaks; that for break shocks platinum contacts are to be preferred to mercury because of their less volatilization, while for make shocks, on account of the rebound or side-slip of metal contacts, mercury affords the only trustworthy contact.

It is, of course, wholly undesirable to equip the primary circuit with two keys, — one of mercury to be used for making the circuit, and another of platinum for breaking it. I shall describe, therefore, an automatic

make and break key with mercury contacts which has been proved by several years' experience to give uniform breaks and makes.*

The key consists of a block of vulcanite 30 mm. long, 20 mm. wide, and 25 mm. deep, having cut in it two vertical chambers (see Fig. 11), one (a) rectangular, 20 mm. long, 8 mm. wide, and 20 mm. deep; the other (b) cylindrical, 6 mm. in diameter and 20 mm. deep. A hole, c (Fig. 11), 3 mm. in diameter, is bored through from one of these cavities to the other at

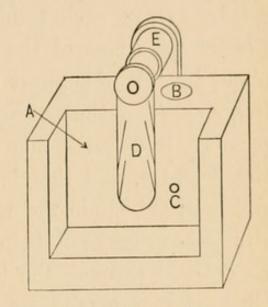


Fig. 11. Diagram illustrating the principle of the vulcanite knife-blade key. The front of the block is broken away to show the relations of the parts within the chamber, a. a and b, mercury chambers; c, opening between a and b; d, vulcanite knife blade supported upon axis, o, which rotates within collar, e.

a depth of about 16 mm. Each of the chambers is in electrical communication with a binding post, and when filled with mercury they are in electrical communication with each other through the connecting hole, c.

^{*} Martin: Am. Jour. of Physiol., 1910, xxvi, p. 181.

A strip of vulcanite, d (Fig. 11), 18 mm. long, 8 mm. wide, and I mm. thick, flat on one side and on the other tapered toward the edges, is supported at the top of the block by a horizontal rod working freely in a collar, e (Fig. 11), in such fashion as to press closely against the inner surface of the cavity, a, and when rotated about its axis of support to cover or uncover the opening, c. When the vulcanite strip is brought over the opening, it cuts the mercury connection between cavities a and b, and therefore breaks any electric circuit which may include them. This method of breaking a circuit has many points in its favor. The break cannot be delayed through the tendency of mercury drops to cling together, for the severance of the mercury column is not the withdrawal of one mass of mercury from another, but is the forcible interposition of a nonconductor in the path.* Moreover, the vulcanite strip cuts off not only the liquid mercury, but if it fits tightly, as it should, cuts off as well any mercury vapor that may be formed. Thus the effect of volatilization of mercury is minimized. Since the point where the break occurs is beneath a considerable depth of mercury, air does not have access to it, and oxidation does not occur. I have found, as a matter of fact, that the same mercury may be used in one of these keys for months without any appreciable variation in the effectiveness of the break.

^{*} A device employing the same principle was described by Lombard in 1902: Am. Jour. of Physiol., 1902, viii, p. xx.

When the vulcanite strip is so rotated as to uncover the hole, c, the mercury in the two cavities reunites and thus makes the circuit. The reunion of the separated mercury masses should take place as smoothly as possible. To bring this about, the vulcanite knife blade is tapered at the edges so that it may plough through the mercury with as little disturbance as possible.

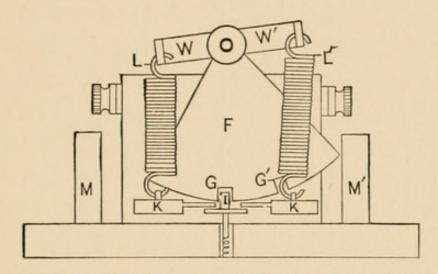


FIG. 12. Diagram of the operating device for the knife-blade key; vertical view. f, triangle of brass bearing slits, g, g', and wings, w, w', rotating about axis, o; l, l', actuating springs; k, k', levers for bringing tension upon springs, and at the same time operating release, i; m, m', stops for limiting motion of knife blade.

The Operating Device. To secure uniformity of action the vulcanite blade must be operated automatically, hand operation being liable to wide variations in the speed with which the contact is made or broken. The method adopted in this instrument is illustrated by the diagrams (Figs. 12 and 13). The axis of rotation of the blade, o (Figs. 11 and 12), after passing through the

supporting collar, e (Fig. 11), is fastened into a triangular sheet of brass, f (Fig. 12), from whose apex project horizontally two brass arms, w and w'; these are

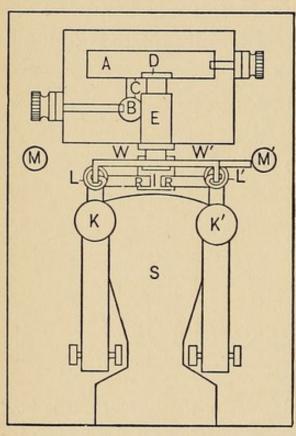


Fig. 13. Diagram of the operating device for the knife-blade key; horizontal view. Significance of letters the same as in Figs. 11 and 12. s, cavity in base for holding short-circuiting device.

bent at right angles at their outer ends, as shown in Fig. 13. From the tip of each of these arms a coiled spring, l and l' (Fig. 12), extends down to the end of a lever, k and k'. Each spring consists of twenty-seven turns of spring brass wire, o.6 mm. in diameter. The length of the spring is about 16 mm., and the outside diameter of the coil 5 to 6 mm. The depression of either lever puts the spring connecting with it under tension and tends to draw downward the correspond-

ing arm, rotating the vulcanite blade with it. To prevent movement of the blade until the spring has been put under a certain degree of tension, two slits, g and g', are cut into the lower edge of the triangle, f. A releasing device, i, is pressed upward against the lower

edge of f by a stout spring, in such fashion that when either slit is engaged f is prevented from moving. Each of the levers, k and k, bears at its tip an arm, r, r' (Fig. 13), which presses upon the releasing device, and when the lever is depressed to a certain point disengages it, allowing the blade to rotate. The amount of motion of the blade is limited by setting two posts, m and m', at such positions that the lower apices of f strike them when sufficient movement has occurred.

After experimenting with various operating devices the one described above has been adopted as combining the greatest number of desirable features with the fewest defects. The two levers, k and k', which are depressed alternately for making and breaking the circuit, are so placed as to lie naturally under the first and second fingers of either the right or the left hand. The springs, l and l', need not be stiff, hence little pressure need be exerted upon the levers, and there is correspondingly little fatigue from continuous operation of the key. The springs are brought under tension only during the use of the instrument; when it is not in use, they hang free. Thus their stiffness does not vary with the lapse of time, as would be the case were one or the other under constant tension.

The Short-circuiting Device. A desideratum in any key which is to be used for stimulating tissues with single induction shocks is a device for short-circuiting auto-

matically either the make shocks or the break shocks at the will of the operator. The instrument under consideration lends itself so readily to the incorporation of

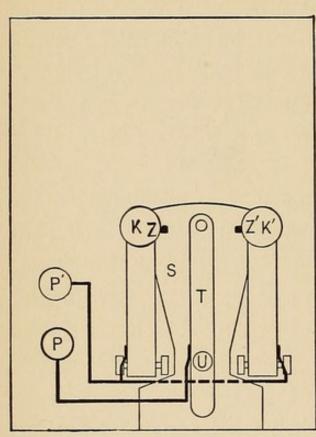


Fig. 14. Diagram of the short-circuiting device. t, brass bar, rotating horizontally about axis, u, and bearing mercury cup, o, which is in electrical communication with post, p. z, z', platinum pins mounted upon levers, k, k', and in electrical communication with post, p'.

such a device that I shall include a brief description of one, believing that the value of the key is enough enhanced thereby to justify its inclusion. The entire mechanism, shown in ground plan in Fig. 13, is mounted upon a slab of vulcanite, which in turn rests upon a base of soapstone, slate, or other suitable material. The vulcanite is cut away between and underneath the levers, k and k', as indicated at s (Fig. 13). A brass rod, t (Fig. 14), is mounted upon an axis, u, in such

fashion that it can be rotated horizontally about this axis within the confines of the space, s. At the end of the rod is a mercury cup, o. Two binding posts, p and p', stand

at one margin of the base. From p a wire leads through the body of the vulcanite block to the rod, t, to which it is soldered near the axis of rotation of the rod. From p' two wires are carried through the block, one to the axis of rotation of the lever, k, to which it is soldered, the other to the axis of k', where it is soldered likewise. Thus both levers are in electrical connection with the post, p', and the rod, t, in similar connection with the post, p. Soldered to the levers, k and k', at the points, zand z', are pins of platinum projecting downward. These pins are so placed that the mercury cup, o, can be brought directly below one or the other of them according as t is rotated. Their length is so adjusted that the pin dips into the mercury when the lever is depressed enough to release the mechanism, but is clear of the mercury at all other times.

If the binding posts, p and p', are connected in parallel into the secondary circuit of the inductorium and the rod, t, is rotated so as to bring the mercury cup below the lever which is pressed when the primary circuit is made (the left-hand one in this instrument) the make shocks are all short-circuited. Bringing the mercury cup below the other lever short-circuits all the break shocks. When the rod is placed in an intermediate position, neither makes nor breaks are affected. To prevent all possibility of accidental diversion of the secondary current into the hand of the operator, vulcanite shields are

placed on the levers at the points where the fingers press upon them, and upon the handle by which the rod, t, is rotated.

In addition to its applicability for both make and break shocks this key has the advantage of preserving uniformity of action for a long time with little attention. In this respect it is superior even to platinum contact keys, which, as is well known, suffer from oxidation after prolonged use. There is no doubt, however, that well made automatic platinum-contact keys, properly looked after, give break shocks of sufficient uniformity for the general purposes of the physiologist.

CHAPTER X

THE INFLUENCE OF SECONDARY RESISTANCE AND OF CATHODE SURFACE

In the preceding chapters the scheme for measuring break shocks has been developed to the point where it becomes necessary to turn from the induction apparatus to the tissue to be stimulated and to inquire how variations in the tissue may modify stimulation strengths. Two possible modifying factors have been indicated (p. 14), as due to variations in the tissue; they are secondary resistance, and the manner of applying the electrodes.

The Relation of Tissue Resistance to Secondary Resistance as a Whole. The secondary circuit usually has a comparatively high resistance. Most inductoria used in physiological laboratories have secondary coils with resistances mounting into hundreds of ohms, and the resistances of the tissues undergoing stimulation are usually high likewise. In numerous determinations of the resistance of stimulated tissues I have met with only one or two under 1000 ohms and have found many exceeding 50,000 ohms.

Since the stimuli imparted by faradic currents as

well as by those of galvanic origin arise from the cathode,* and since the resistance of the physiological
cathodes must be small in comparison with that of the
whole mass of tissue traversed by the current, we are
justified in considering tissue resistance as external to
the actual seat of stimulation, and need make no distinction between this and the other resistances that may
be included in the secondary circuit.

The Method of Experimentation. In studying the influence of secondary resistance experimentally the usual procedure has been to introduce known, non-inductive, resistances into the secondary circuit and to observe the effect of their introduction upon the stimulating value of the shocks sent through the circuit. As a check upon this method some experiments were performed in which different amounts of tissue were included between the stimulating electrodes, and thus the resistance of the tissue itself was varied. This latter method is of course less certain than the former, since the inclusion of more or less tissue in the circuit may mean a variation in the number and irritability of the physiological cathodes involved.

Tissue resistances were determined by means of an ordinary Wheatstone bridge according to the Kohlrausch method, with an alternating current to avoid

^{*} Chauveau: Journal de la physiologie, 1859, ii, pp. 490, 553. See also Biedermann: Elektrophysiologie, Jena, 1895, ii, p. 622.

polarization, and a telephone in place of the galvanometer. Figure 15 is a diagram of the apparatus required. The average of three readings was always taken. This procedure, in the hands of one experienced in its use, gives results accurate within 4 or 5 per cent, a degree of accuracy sufficient for the purposes of this inquiry.

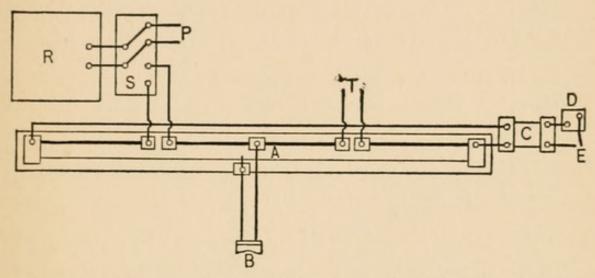


Fig. 15. Diagram of apparatus for measuring tissue resistance. A, Wheatstone bridge; B, telephone; C, small induction coil; D, battery for same; E, key for same; T, wires leading to tissue; R, resistance box connected with switch, S, in such fashion as to be available for use as known resistance of Wheatstone bridge, or as part of primary circuit, P.

Break shocks were used for determining the threshold of contraction. The expression for the value of the stimulus is Z, determined from the formula, $Z = \frac{M}{L}I$.

The Effect upon the Stimulus of Varying the Secondary Resistance. The effect upon the value of Z of varying the secondary resistance is shown in two representative experiments cited in Table VI. As appears

TABLE VI

The Influence of Secondary Resistance upon the Stimulating Values of Induced Currents

Experiment of Dec. 15, 1909. Resistance of Secondary Coil = 1400 ohms; of Tissue = 1700 ohms. Tissue = Frog's Gastrocnemius, Uncurarized.

Resistance	in	secondary	

circuit	3100	6100	10,100	15,100	18,100
Value of Z	4.96	6.81	9.45	12.45	14.1

Experiment of March 1, 1910. Resistance of Secondary Coil = 1400 ohms; of Tissue = 16,600. Tissue = Frog's Sartorius, Uncurarized.

from this table, stronger stimuli are required to produce a given physiological effect when the secondary resistance is high than when it is low. That there is a definite mathematical relationship between the effectiveness of the stimulus and the secondary resistance is shown by plotting these values as a curve. Such a curve for the first experiment of Table VI is given in Fig. 16. It is virtually a straight line having the general equation

$$Z = \frac{\beta \left(R + A \right)}{A},\tag{1}$$

in which Z is the intensity of the shock required at resistance R to produce the desired effect, and β and A

are constants. This formula has been found to hold in all of the several hundred experiments, in which it has been applied. The value of the constant β in any

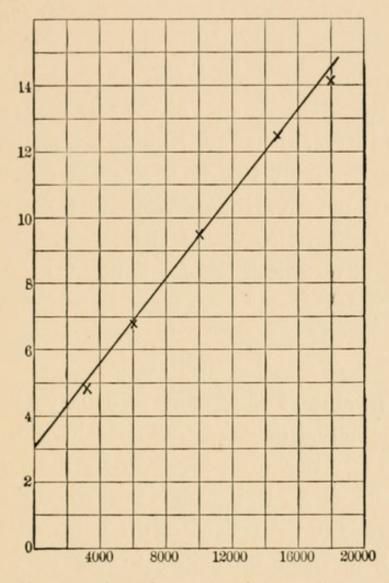


Fig. 16. Showing that the curve of increasing stimulus against increasing resistance is a straight line. Abscissæ represent values of Z; ordinates represent resistances in ohms.

given experiment can be determined geometrically by producing the curve to where it cuts the ordinate for zero resistance. According to Fig. 16, the value of β for the experiment of Table VI from which that curve is derived is 3. Since this represents the value of Z, whose effect at zero resistance would equal that of the various other values of Z at their respective resistances, it affords a measure of the irritability of the physiological cathode where the stimulus actually arose, on the assumption that the resistance of the cathode is negligibly small. We have, therefore, in β an expression for the value of any stimulus as it affects the seat of actual stimulation, namely, the physiological cathode, irrespective of the resistance of the secondary circuit.

By a slight transposition of equation (1) the equation for β becomes:

$$\beta = \frac{ZA}{R+A},\tag{2}$$

and if the value of Z for any secondary resistance is known, the actual or "specific" stimulus can be calculated from equation (2), provided only the value of the other constant, A, is known. For measuring stimuli with reference to the resistance through which they are applied there must be added to the determinations previously required, therefore, not only the secondary resistance, but a constant A.

Current Density an Important Factor. That the stimulating effectiveness of electric currents varies with their density has long been recognized,* although practical

^{*} Biedermann: Loc. cit., 1, p. 185.

application of the fact has hitherto been reserved for galvanic stimulation. The expression for β shows that current density is a factor to be taken into account in measuring faradic stimuli as well.

The factor A in the expression $\beta = \frac{ZA}{R+A}$ is the provision by which allowance is made for the influence of current density. The stimulating effectiveness of dense currents is greater than of diffuse ones. In order that the expression for β agree with this fact the value of A must increase as the density of the stimulating current increases. Experimental evidence showing that A is actually larger for dense currents than for diffuse currents is contained in an experiment cited on p. 109, Chap. XII.

I do not know of any reliable method of determining the value of the constant, A, other than that used in this work, namely to establish experimentally two or more values of Z for different secondary resistances, and from these values compute the value of A. This can be done by means of the equation

$$A = \frac{Z_R R' - Z_{R'} R}{Z_{R'} - Z_R},\tag{3}$$

in which Z_R and $Z_{R'}$ are the stimuli required, with resistances R and R' respectively, to produce the minimal contractions used as the index.

The Dependence of Factor A upon Inductorium Construction. In discussing the method of comparing one inductorium with another by the introduction of the factor L in the expression $Z = \frac{MI}{L}$, it was stated (p. 52) that this comparison is subject to a certain restriction as to secondary resistance. This restriction rests upon an observation of Gildemeister,* according to which, if two dissimilar inductoria are compared quantitatively by the method outlined here, in which the expression for the value of a stimulus is $Z = \frac{M}{L} \times I$, it will be found that although equal stimuli may yield corresponding values of Z from the two inductoria, with certain secondary resistances, when other secondary resistances are used equal stimuli will not give corresponding values of Z.

In earlier paragraphs of this chapter it was pointed out that the true or *specific* value of a stimulus is not afforded by the expression Z, but by the expression β , which depends not only upon Z but upon the secondary resistance and a constant A as well. The determination of A, as previously shown, is according to the formula

$$A = \frac{Z_R R' - Z_{R'} R}{Z_{R'} - Z_R},$$

in which Z_R and $Z_{R'}$ are stimuli which, with resistances

^{*} Gildemeister: Archiv für die ges. Physiologie, 1910, Bd. 131, S. 604.

R and R' respectively, have equal physiological effect. Since dissimilar inductoria fail to give corresponding values of Z at all secondary resistances, the value of A determined by this formula from one inductorium will not necessarily agree with its value as obtained from another. The value of A, therefore, does not depend solely upon the surface of the physiological cathodes, but in part also upon the construction of the inductorium.

This variation in the values of A determined from dissimilar inductoria, which might lead one to question the validity of the equation in which A is employed, i.e.,

 $\beta = \frac{ZA}{R+A}$, serves in fact to confirm strongly the valid-

ity of that equation and the use of the expression β to signify the specific value of the stimulus. This confirmation rests upon the repeated observation that when equal stimuli are generated by dissimilar inductoria the values of β are equal even though the observed values of Z and the computed values of A may be quite divergent. An experiment illustrating this point is summarized in Table VII. Details of the construction of the inductoria used are given in Table VIII. The experiment shows that dissimilar inductoria give for equal break stimuli perfectly concordant values if all the factors which make up the final expression for stimulation strength are taken into account.

TABLE VII

Demonstrating that Equal Stimuli give Equal Values of β in the Equation $\beta = \frac{ZA}{R+A}$, when the Stimuli are generated by Dissimilar Inductoria

Inductorium.	н.	N.	В.
First sec. resistance First Z Second sec. resistance Second Z Calculated A Calculated β	0.76 25,500 ohms 1.60 6,200	0.604	0.588

The differences in secondary resistance in corresponding columns are due to the different resistances of the secondary coils, it being necessary to include these resistances as part of the secondary circuit.

TABLE VIII

Details of Construction of the Inductoria used in this Study

Coil.	Length of secondary.	Turns in sec- ondary.	Resistance of second- ary.	Remarks.
A	cm. 12.5	10,000	850	Kronecker graduation
В	13.0	10,350	1400	Kronecker graduation
G	13.0	10,260	770	Kronecker graduation
E	6.5	5,000	300	Porter inductorium
H	9.3	6,000	450	
N	9.3	8,000	600	

Conditions in which the Specific Stimulus need not be determined. While we have in the formula $\beta = \frac{ZA}{R+A}$

a means of expressing the specific value of any break induction shock, no matter how the factors concerned in its production may vary, we must recognize that in the ordinary practice of the physiologist the attempt to make use of this formula presents very considerable difficulties. These difficulties, moreover, are chiefly in connection with the inclusion of the factors R and A, and we may well inquire how great errors are likely to arise in comparing faradic stimuli if these two factors are completely disregarded.

We must realize at the outset of this part of our inquiry that if comparisons are attempted between stimuli used under conditions of widely varying secondary resistance and divergent cathode surface, disregard of these two factors is sure to lead to erroneous conclusions; but probably in a majority of physiological experiments the stimuli to be compared are produced under conditions which tend to be closely similar. With regard to such cases as these we may properly inquire whether the factors under consideration need be taken into account.

Successive Stimulation of the Same Tissue. Probably the experiments in which accurate comparisons of stimuli are most needed are those in which a given tissue is to be stimulated successively. But in experiments of this class neither the tissue resistance nor the electrode surfaces undergo noteworthy variation during the course of the experiment and so do not enter as modifying factors.

Stimulation of Corresponding Tissues in Different Animals. Next in importance are cases in which it is desired to impart comparable stimuli to corresponding tissues through a series of experiments. Cases of this sort arise frequently in the course of physiological research, and I have therefore given them special consideration.

While this subject was before me there was being carried on in the laboratory at Harvard an investigation which involved, among other things, determining in a series of cats the threshold stimulus for producing extension of the wrist, when the stimulus was applied to the deep branch of the radial nerve below the elbow; and reflex flexion of the hind leg through stimulation of the tibial. Here was presented a typical example of the class of experiments described in the paragraph heading, and I therefore utilized it in the study of my problem. In several cases the threshold stimulus was determined when the tissue only was in the secondary circuit, and immediately afterward, the threshold when an additional resistance of 10,000 ohms had been introduced. I was thus able in these cases to compute the value of the constant A, and from it to obtain the solution of the equa-

tion for "specific" irritability, $\beta = \frac{ZA}{R+A}$. In the ex-

periments of this series, ten in all, the secondary resistances ranged from 2800 ohms to 6000 ohms, averaging 3900 ohms. The values of A ranged from 4300 to 14,000, averaging 7800. The statistics for this series are given in Table IX.

TABLE IX

Illustrating the Tendency of β and Z to vary similarly in Direction and Extent. Z represents the Stimulus producing Just Perceptible Wrist Extension in Cat. Stimulus applied to Deep Branch of Radial Nerve

Date, 1910.	Secondary resistance.	Value of A.	Value of Z.	Value of β.	Ratio $\frac{\beta}{Z}$.
Aug. 8. July 28. Aug. 5. Aug. 3. Aug. 9. Aug. 2. Aug. 17.	6000 4400 4800 3400 3000 4600 2800	7500 5000 8000 7800 9800 9600 4600	2.77 3.19 3.84 4.32 5.52 6.05	The second secon	.56 .53 .62 .70 .77 .68

As Above except that Stimulus was applied to Tibial Nerve, and Reflex Flexion of Hind Leg was Movement Evoked

July 18	4000 3000	4,300 14,000 7,000		5.1	· 59 · 77 · 70 · 65
---------	--------------	--------------------------	--	-----	------------------------------

Inspection of the table reveals a definite tendency of β to vary as does Z. The closeness of this tendency is brought out more strikingly, however, in Fig. 17, in

which the ratios of β to Z in successive experiments are plotted. The horizontal line represents the average ratio of β to Z as determined in these experiments; the variations from this line of the different actual ratios are, as is seen, relatively inconsiderable, the greatest being 18.5 per cent, the average of all slightly under 11 per cent.

Assuming the data cited in Table IX to be fairly representative of the relations between β and Z that are

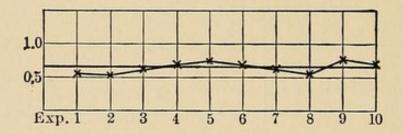


Fig. 17. Illustrating the relatively slight departures of individual ratios of β to Z from the average. Ordinates represent successive experiments; abscissæ represent ratios of β to Z. The horizontal line is drawn at the level of the average ratio.

likely to occur in experiments of the sort under consideration, to what extent are we justified in such experiments in making use of the values of Z for expressing quantitative relationships?

The figures show clearly, I think, that all except the finest relationships are revealed with sufficient exactness by the values of Z. While one cannot always know certainly, in cases in which several nearly equal values of Z are under comparison, which will give smaller and

which larger values of β , yet, if the experiments are carefully performed, one can be practically certain, whenever the values of Z differ by more than 15 or 18 per cent, that the larger Z means also a larger β . With this degree of accuracy assured, probably the demands of most researches of this class are fully met, and all such may safely disregard both the secondary resistance and the cathode surfaces.

Differing from the series of experiments quoted above in that they offer wider variations in both secondary resistance and electrode surface, and therefore greater likelihood of error if these factors be disregarded, is a series of observations on frogs' gastrocnemius muscles, carried out by myself.

In the series of eighteen experiments cited in Table X the secondary resistances ranged from 3100 to 13,000 and the values of A from 2600 to 13,500. Yet, in spite of these wide ranges in the values of the factors determining the relation of Z to β , this latter relation varies to a surprisingly moderate degree. The average ratio of β to Z is .49. The widest departures from this are ratios of .32 and .64, amounting to 35 per cent and 31 per cent respectively, while the average variation is only 15 per cent. If the experiments of Table X represent fairly the variations in secondary resistance and cathode surface likely to be met with in experiments on frogs' gastrocnemii, we can safely conclude that the values of Z, obtained in any such experiment, represent the true relative values of the stimuli used within one-third.

TABLE X

Illustrating Tendency of Z and β to vary together. Frogs' Gastrochemii stimulated directly

Date.	Secondary resistance.	Value of A.	Value of Z.	Value of β.	Ratio $\frac{\beta}{Z}$.
Feb. 24, 1910. Oct. 28, 1909. Dec. 15, 1909. Jan. 19, 1910. Feb. 17, 1910. Feb. 24, 1910. Feb. 18, 1910. Jan. 31, 1910 Mar. 7, 1910 Feb. 18, 1910 Nov. 18, 1909. Feb. 10, 1910. Jan. 31, 1910. Dec. 13, 1909. Jan. 31, 1910. Feb. 18, 1910. Feb. 18, 1910. Feb. 18, 1910. Feb. 17, 1910. Nov. 4, 1909. Average.	5,400 6,500 3,100 8,400 6,800 6,400 5,000 11,400 5,400 5,500 7,700 13,000 10,400 5,000 6,200 5,000 6,000 3,200	6,900 6,000 5,000 4,800 7,500 4,200 4,800 13,500 4,800 5,500 4,200 6,000 9,000 5,000 10,500 4,800 10,500 2,600	6.12 6.24 11.9 12.2 12.35 12.5 12.7 12.95 14.6 14.6 15.35 16.8 19.2 19.9 22.1 22.8 24.7 41.5	3.4 3.0 7.35 4.45 6.5 4.95 6.2 7.0 6.86 7.3 5.40 5.30 8.90 9.96 13.9 11.2 15.7 18.6	.56 .48 .62 .36 .52 .40 .49 .54 .47 .50
		1/3			

In a series of ten experiments on frogs' gastrocnemii stimulated through the sciatic, with resistances ranging from 6300 to 38,000 ohms, and values of A from 6000 to 23,000, the ratio of β to Z averaged .48, and the widest variation was a ratio of .28, amounting to 42 per cent, the average variation being 20 per cent. In the experiments cited in the two series above no attempt was

made to keep conditions of tissue resistance and cathode surface approximately uniform. On the contrary, these conditions were purposely made to vary widely from one experiment to another. I feel, therefore, that they cover the range of variation likely to occur in ordinary experimentation.

These data seem to me to show that in the hands of a careful experimenter, who will take pains to keep his conditions of stimulation as uniform as possible, quantitative results of great value may be obtained without the labor involved in taking account of secondary resistance and cathode surface. By the use of the method outlined in previous chapters the strengths of stimuli employed in any given case may be expressed in terms of stimulation units, and if the conditions of experimentation, such as the nature of electrodes used, distance between them, and method of applying them, are carefully described, other experimenters can duplicate the stimuli very closely. Certainly this method allows comparisons of much greater accuracy than can be made by the existing methods of describing stimuli. It is highly important, however, that investigators attempting to use induction shocks quantitatively recognize fully the limitations upon accuracy which are involved in disregarding the factors under discussion. So long as there is no effort to draw conclusions which are not warranted by the degree of accuracy actually obtained, no harm will be done, but wherever the occasion exists for a high degree of accuracy in determining stimuli, secondary resistance and cathode surface must be taken into account.

A Standard of Inductorium Construction Necessary. In connection with this discussion of the circumstances in which the factors of secondary resistance and cathode surface may be disregarded, we must not forget that the structure of the inductorium is interwoven with the factor of cathode surface (see p. 78), in such fashion that the latter cannot be left out of account without error unless the former has been provided for. This provision is best made by adopting a standard of inductorium construction and using for quantitative purposes only instruments conforming reasonably to it. Thus we become at once independent of inductorium structure as a complicating factor, and are free to measure stimuli in many cases in the simpler manner discussed above.

The desirability of having a standard of inductorium construction for physiological and clinical use was recognized fully thirty years ago. In an attempt to establish one the Paris Electrical Congress of 1881 resolved at its session of September 28th that the form of inductorium at that time in use in the University of Berlin should be adopted as the standard.*

^{*} See Lewandowski: Elektrodiagnostik und Elektrotherapie, Wien und Leipzig, 1887, S. 212. Also Hoorweg: Die medicinische Elektrotechnik und ihre physikalischen Grundlagen, Leipzig, 1893, S. 128.

The dimensions of that inductorium are as follows:

	Primary	Secondary
Length of coil	88 mm.	65 mm.
Diameter of coil	36 mm.	68 mm.
Diameter of wire	ı mm.	0.25 mm.
Number of turns of wire	300	5000
Number of layers of wire	4	28
Resistance	1.5 ohms	300 ohms

Unfortunately for the general acceptance of these dimensions as standard, Kronecker * had, ten years earlier, proposed his well-known system of units, based on determinations made with inductoria having coils twice as long as the Berlin coils and each with twice as many turns of wire; and with the adoption of his graduation the large coils came into common use. By general consent among physiologists, therefore, rather than by any official action, inductoria having coils about 13 cm. long and having about 10,000 turns in the secondary are recognized as suitable for the uses of the investigator. In most well-equipped laboratories such inductoria are found, and there seems no valid reason why the general dimensions originally selected by Kronecker for his graduation should not be taken as standard. In a later paragraph (p. 92), observations will be cited which show that for quantitative work coils of this size are to be pre-

^{*} Kronecker: Arbeiten aus der physiologischen Anstalt zu Leipzig, 1871, S. 186.

ferred to the smaller ones recommended by the Paris Congress.

Assuming as the standard, then, an inductorium having coils about 13 cm. long and having in the secondary approximately 10,000 turns of wire, we may inquire how widely an inductorium can vary from this standard without introducing a significant error. For answering this question I have made observations with six inductoria, three of which are of "standard" construction and provided with Kronecker graduations, the other three selected to give increasing degrees of divergence from the standard. Details of the construction of the six inductoria are set down in Table VIII.

The results of my numerous experiments with these inductoria may be summarized as follows: The three standard coils, A, B, and G, give corresponding values of Z for equal stimuli and equal secondary resistances whatever the secondary resistance may be. In comparing them, therefore, the factor of inductorium construction does not enter.

In thirteen experiments in which coil N was compared with coil B the secondary resistances ranged between 2850 ohms and 25,000 ohms; the average percentage variation of Z_N^* from Z_B was 6 per cent; the greatest variation was 11.6 per cent. Z_N was greater than Z_B

^{*} For convenience of expression a subscript is placed after the value of Z to indicate with which coil the value was obtained.

QI

four times and Z_B greater than Z_N nine times. The small average percentage difference between the two coils, a difference only slightly greater than the probable experimental error, coupled with the fact that not all the variations are in the same direction, seems to me to show that in coils differing no more than these the influence of inductorium construction as a special factor can be disregarded without serious error.

An important effect of inductorium construction becomes manifest when coils B and H are compared. The average difference between Z_B and Z_H in twelve experiments was 16 per cent; in four of the twelve cases, moreover, the difference exceeded 24 per cent. Analyzing the series of experiments with reference to the secondary resistances it appeared that the high average difference is due to large differences in the experiments with high secondary resistance. Thus five experiments with secondary resistance above 10,000 ohms show an average difference between Z_B and Z_H of 25.7 per cent, while seven experiments with secondary resistances below 10,000 ohms show an average difference of only 4.5 per cent. In all five experiments with high secondary resistance Z_H was greater than Z_B . In the seven experiments with low resistance Z_H was larger than Z_B three times, smaller than Z_B twice, and equal to it twice.

This series of experiments shows that in inductoria differing even so widely as do coils B and H, inducto-

rium construction is unimportant so long as secondary resistance is kept low. It is, however, of great importance whenever the secondary resistance is high.

The final series of comparisons was between coil B and the Porter inductorium, coil E. This yielded results of the same sort as the preceding comparison, but more marked. Only with very low secondary resistances were Z_B and Z_E equal, and Z_E became relatively more and more in excess of Z_B as the secondary resistance was increased. Table XI illustrates this relationship very clearly.

This last experiment brings out clearly the objection to the standard set by the Paris Congress of 1881

TABLE XI
Illustrating the Increasing Divergence of Z_E from Z_B with Increasing Secondary Resistance

Resistance in sec- ondary circuit.	Z_B .	Z_E .	Percentage variation of Z_B from Z_E .
900 ohms	15.75	16.05	1.9
1,600 ohms	17.9	19.8	10.6
2,700 ohms	18.7	26.8	43.0
8,600 ohms	24.1	46.0	91.0
20,600 ohms	49.0	135.0	175.0

(p. 89). The Porter inductoria conform closely to that standard in all respects save that of diameter of the coils. As Table XI shows, the influence of secondary resistance upon stimulating value is very much more marked in

the small inductorium than in the larger one, so that while there are many sorts of experiments in which the investigator using a large coil is justified in disregarding secondary resistance, to do so would nearly always be unsafe if a small coil were being employed.*

* The Porter inductorium with which this experiment was performed is of the old, or student, type. The new form, which is constructed in accordance with the Kronecker specifications, is well adapted for quantitative work.

CHAPTER XI

THE MEASUREMENT OF MAKE SHOCKS

In order that the scheme for making induction shocks quantitatively useful may be complete, a method for measuring make shocks must be added to the one already developed for break shocks. The method to be presented in this chapter is based wholly on experimental comparisons between make shocks and break shocks by the v. Fleischl method previously described (p. 56). That it is valid can scarcely be doubted in view of the large number of concordant experiments which support it.*

The expression for make shocks should, of course, be directly comparable with the one previously developed for break shocks. The factors of secondary resistance and cathode surface affect makes and breaks alike. We may take as a starting point from which to develop a formula for make shocks, therefore, the expression for break shocks which takes account of neither of these factors, namely $Z = \frac{MI}{L}$. The problem to be solved is how this expression must be modified so that the value

^{*} Martin: Am. Jour. of Physiology, 1909, xxiv, p. 276 et seq.

Z as applied to make shocks shall represent stimuli equal in intensity to those given by break shocks in which the value of Z is determined as above. The experimental procedure by which the problem was solved was as follows: A series of equal make stimuli were obtained with the secondary coil at various distances from the primary. The "calibration number" for each secondary position was then multiplied by the intensity of primary current employed at that position, and the products for each experiment were set down in a table.* For the inner positions of the secondary coil, positions which have relatively large values of $\frac{M}{L}$, the product $\frac{M}{I} \times I$ was nearly constant; as the secondary coil was moved out into the parts of the field where the values of $\frac{M}{I}$ are small, the product $\frac{M}{I} \times I$ became progressively larger the farther out the secondary coil was pushed, and consequently the smaller were the values of $\frac{M}{I}$. Numerous repetitions of the experiment gave precisely similar results.

These experiments indicated quite clearly the existence of a comparatively simple relationship between make and break stimuli, and also suggested a method

^{*} For experimental data see Martin: Loc. cit., p. 272.

for expressing the relationship mathematically in the simplest possible fashion, namely through the introduction of a single factor into the break shock formula, which when introduced would cause it to give equal values for Z for equal make stimuli. Study of the data showed that the factor to be introduced must be relatively larger the smaller the value of $\frac{M}{L}$, and must tend to diminish $\frac{M}{L}$. A constant number has this effect

if it is subtracted from $\frac{M}{L}$. The formula modified in accordance with this idea becomes

$$Z_m = \left(\frac{M}{L} - K\right)I.* \tag{1}$$

In practically every experiment of a large series some number could be selected to be substituted for K in formula (1) with a fairly constant value of Z resulting. For each experiment the value of K had to be determined empirically, and it varied widely in different experiments. In all the experiments the values of K were negligibly small in comparison with the values of $\frac{M}{L}$ for secondary positions of 12 cm. or less.

The discovery of the above formula is a decided step toward the ultimate solution of the problem of measur-

^{*} To distinguish between break stimuli and make stimuli the former are represented by Z_b , the latter by Z_m .

ing make shocks, but it is not a complete solution, since it offers no means of determining in advance what the value of K will be under any given set of conditions. The next step was to study a large series of experiments with reference to the conditions upon which the values of K depend.

It became apparent at an early stage of the investigation that make shocks, unlike breaks, are modified in intensity by changes in the voltage of the primary current. This observation suggested the grouping of all the experiments according to the primary voltage used in performing them. After this had been done the values of K for the different experiments of any group still differed widely, but now wherever the value of K was large the value of Z was also large and $vice\ versa$. This suggested at once a possible dependence of the value of K upon that of Z. To test this possibility the experiments of each group were plotted, values of K against values of Z. The resulting curve in each case is a straight line, having the simple equation

$$K = aZ. (2)$$

Fig. 18 gives the curve for coil B obtained by plotting the experiments at 2 volts. The value of a given by this curve is 18. Substituting in equation (1) the value of K given in equation (2), we have

$$Z_m = \frac{M}{L}I - aZI. (3)$$

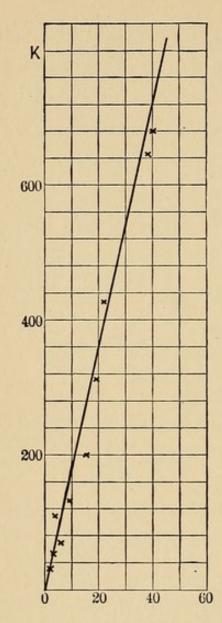


Fig. 18. Curve obtained when the values of Z given by the application of the formula $Z = \left(\frac{M}{L} - K\right)I$ to the experiments performed with a primary voltage of 2 are plotted against the values of K used in these experiments. Abscissæ represent values of K; ordinates represent values of K. The equation for this curve is K = 18 Z.

This solved for Z_m and simplified gives

$$Z_m = \frac{\frac{M}{L}}{\frac{1}{I} + a}, \qquad (4)$$

an equation which enables us to determine the value of make stimuli at any given primary voltage, for which the value of a is known.

There remains now for the completion of the make shock formula only the establishment of a definite relationship between the values of a at various primary voltages and the voltages themselves. To determine whether such a relationship exists another curve was plotted, primary voltages against values of a previously determined. This curve is represented in Fig. 19. It has the


simple equation

$$E = a \cdot C, \tag{5}$$

in which C represents a constant. Substituting in equation (4) the value of a given by equation (5), we have

$$Z_m = \frac{\frac{M}{L}}{\frac{1}{I} + \frac{C}{E}}, \qquad (6)$$

which is the general equation for make induction shocks. The value of C is fixed Fig. 19. Curve obtained by plotting for each inductorium. For the one with which this equation was developed, coil B, its value is 36.

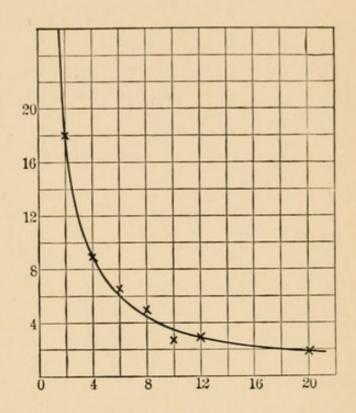

against the different primary voltages used in these experiments the values of a obtained from curves plotted as in Fig. 1. The equation for this curve is $E \times a$ = 36. Abscissæ represent values of a; ordinates represent primary voltages.

Comparison of the General Formulæ for Break and Make Stimuli. If the general equation for break shocks be written in the same form as the one for make shocks and the two placed side by side, the simple mathematical relationship existing between make and break stimuli becomes apparent. Written thus, the break shock 100

formula is

$$Z_b = \frac{\frac{M}{L}}{\frac{\mathrm{I}}{I}}.$$

Comparing this with the make shock formula,

$$Z_m = \frac{\frac{M}{L}}{\frac{1}{I} + \frac{C}{E}},$$

the difference between them is seen to be wholly in the denominator, and to consist of the addition of a simple expression to the denominator of the break shock formula to give the one for make shocks. Inasmuch as increasing the denominator of a fraction diminishes the value of the fraction, the formulæ express the well-known fact that make shocks are weaker than break shocks produced under equivalent conditions.

In the formulæ as here presented the numerators express the influence upon the value of Z of the position of the secondary coil with respect to the primary. The denominators express the influence upon Z of the intensity of the primary current, and for make stimuli the influence of its voltage also. Since the numerator is the same in both formulæ, i.e., $\frac{M}{L}$, it follows that how-

ever the break stimulus Z_b may compare with the make stimulus Z_m , changing the value of $\frac{M}{L}$ by moving the secondary coil does not affect the relationship between them. To illustrate, if we suppose the break stimulus to be twice as intense as the make stimulus when the secondary coil is at zero, the break will continue to be twice as intense as the make wherever the secondary coil is placed, provided, of course, that all other conditions remain constant.

Since the difference between the two formulæ is wholly in their denominators, we may expect careful analysis of these to yield a full understanding of the conditions upon which depend the relationships between make and break stimuli. The denominator of the make shock formula will always be larger than that of the break formula, but the amount of difference between the two will vary greatly according to the relative values of $\frac{1}{I}$ and $\frac{C}{E}$. This can best be shown by a concrete case. Let us first compare the values of Z_b and Z_m in a hypothetical experiment with coil B in which a primary current of 0.0005 ampere at 20 volts is employed. The expression for Z_b is

For Z_m the expression is

$$\frac{\frac{M}{L}}{\frac{2000 + \frac{36}{20}}{1000}} = \frac{\frac{M}{L}}{\frac{2001.8}{1000}}.$$

The difference between the stimulating intensities of the two sorts of shocks is in this case less than one-tenth of one per cent. Compare now the values of Z_b and Z_m when a primary current of 0.4 ampere at 2 volts is used. The

expression for
$$Z_b$$
 is $\frac{M}{L}$,

and for Z_m is

$$\frac{\frac{M}{L}}{2.5 + \frac{3.6}{2}} = \frac{\frac{M}{L}}{20.5}.$$

In this case the break shock is more than eight times as intense as the make.

The above illustrations present in concrete form the effects upon the relation between break and make stimuli of variations in intensity and voltage of the primary current. These effects may be stated in general thus: The higher the voltage of the primary current and the less its intensity, the more nearly will make shocks equal break shocks: conversely, the lower the voltage of the primary current and the greater its intensity, the more will break shocks exceed make shocks.

The make shock formula shows that make stimuli do not vary directly with the intensity of the primary current as break stimuli do. Although make shocks increase absolutely with every increase in primary intensity, other conditions remaining uniform, the increase is relatively slight when primary intensities of considerable magnitude are compared. For example, if with coil B a 2 volt primary current be increased from 0.5 ampere to 1.0 ampere, the make stimuli will be increased only 5 per cent, while break shocks under the same circumstances would be doubled.

This peculiarity of relation of make shocks to primary currents of high intensity shows itself very strikingly in many experiments in which minimal muscular contractions are used as indicators of stimulation strength. In the outer parts of the field of the inductorium, where the

values of $\frac{M}{L}$ are small, primary currents of high intensity

must be employed to give shocks sufficient to elicit visible response. I have often found when studying make shocks, especially with primary currents of low voltage, that as the secondary coil was pushed out to a point where primary currents of 0.1 or 0.2 ampere failed to elicit response, no increase of primary intensity up to the limits of my apparatus would raise the stimulus to the threshold. This frequent failure of relatively enormous primary currents to give detectable make stimuli

was wholly inexplicable until the development of the make shock formula made its meaning clear.

Although the make shock formula

$$Z_m = \frac{\frac{M}{L}}{\frac{1}{I} + \frac{C}{E}}$$

presents the appearance of some complexity, as a matter of fact it is a comparatively easy task to derive the value of C, which is the only new constant the equation requires, and with the constant once established the use of the formula is perfectly simple. To determine how laborious is the task of determining the value of C, an inductorium was taken which had been previously calibrated for break shocks, and seven experiments were found to yield sufficient data to establish conclusively the value of the constant.

The experimental procedure is that described on p. 95. The interpretation of the results so as to establish the constant depends upon recognition of the fact that in such experiments as these the value of Z_m for the inner positions of the secondary coil, where threshold stimulation is obtained with very small primary currents, is practically independent of the value of the constant; whereas the value of Z_m for secondary positions far out on the scale, where heavy primary currents must be

used, can be correctly determined only if the constant is accurately known.

By transposition of the equation

$$Z_m = \frac{\frac{M}{L}}{\frac{1}{I} + \frac{C}{E}},$$

we obtain the formula for the constant

$$\frac{C}{E} = \frac{\frac{M}{L}}{Z_m} - \frac{\mathbf{I}}{I}.$$
 (7)

By taking advantage of the fact above noted, that the value of Z_m for the inner secondary positions is independent of C, we can obtain Z_m for any given experiment by taking the product of $\frac{M}{L} \times I$ for these positions. Since the value of Z_m is assumed to be constant throughout the experiment we can apply this value to the solution of equation (7), using the data obtained at the outer secondary positions to give $\frac{M}{L}$ and $\frac{1}{I}$. From four experiments at 2 and 4 volts were obtained by this method the following values of C: 8.16, 8.0, 6.8, 9.0, 8.0, 9.8, 8.0, 5.2, 8.0. The average of these is 7.9. The nearest round number, 8, was taken as a sufficiently close approximation to the constant, and was applied to three other experi-

ments at primary voltage ranging from 2 to 12. When so applied, constant values of Z_m were obtained,* thus proving the correctness of the determination.

* For data see Martin: Amer. Jour. of Physiology, 1909, xxiv, pp. 279 and 280.

CHAPTER XII

ERRORS TO BE AVOIDED

Incidental results of the several years of study spent in developing the quantitative method here presented have been to emphasize the importance of certain precautions, and also to reveal the errors committed by some users of induction shocks in their efforts to make quantitative comparisons by indirect methods.

Probably the most urgent general precaution calling for discussion is that of maintaining good electrical contacts throughout. In a mechanism so complicated as that shown in Fig. 8 loose contacts which may easily escape observation are likely to render quantitative observations completely valueless. The user of the apparatus must keep continually in mind the importance of maintaining tight contacts, and by frequent inspection must assure himself that they are so. The sliding contacts provided for the secondary coils in some forms of inductoria are very untrustworthy and should not be used if fixed ones are available.

In applying stimulating electrodes one must have in mind that the induced current stimulates at the *cathode*, and must know which electrode this is. A simple means of distinguishing the poles of the secondary circuit is to apply them to a sheet of filter paper moistened with a mixture of starch paste and potassium iodide solution. If a strong primary current is made and broken rapidly, and the secondary makes or breaks are short-circuited each time, a blue deposit presently appears at the anode, indicating the accumulation there of iodin ions which react with the starch. It should be remembered that make shocks and break shocks are opposite in direction, so that the pole which is revealed as the anode for break shocks is the cathode for makes.

The development of a mathematical expression for the influence of secondary resistance on stimulating value has shown the fallacy of a method sometimes employed for varying stimulating strengths quantitatively by including known resistances in the secondary circuit and assuming that the strength of stimulus is reduced in exact proportion with the increase of resistance. As the equation (p. 76) shows, the strength of stimulus not only does not vary in exact proportion with the resistance, but the relationship actually existing is not apt to be the same in two successive experiments, owing to the interrelation between secondary resistance and cathode surface.

This same interrelation explains the error of another procedure which has sometimes been employed for the purpose of overcoming inequalities in stimulation strength due to differences in secondary resistance, namely the introduction of a very high additional resistance into the secondary circuit, thereby making fluctuations in tissue resistance relatively negligible.— That this device is perfectly adequate in experiments in which a single tissue of varying resistance is under examination is of course obvious; there being under such circumstances no variation in cathode surface. But in experiments in which different tissues are being compared the introduction of high additional resistance into the secondary circuit is more apt to be misleading than otherwise because of the cumulative effect of variations in cathode surface. The point can best be illustrated by a concrete example:

Experiment of March 7, 1910. - Frog's gastrocnemius muscle stimulated directly. In the first test the cathode was in contact with the surface of the muscle, but did not penetrate it. When the tissue only was in the secondary circuit, the total secondary resistance was 17,000 ohms. A minimal contraction was secured with a value of Z equal to 6.6. When 70,000 ohms' additional secondary resistance was introduced, the value of Z was 16.8. By calculation the value of A was found to be 28,000, and that of the specific stimulus β to be 4.1.* In the second test the cathode was thrust directly through the muscle tissue; the secondary resistance was 5400 ohms; the value of Z was 6.1. When 70,000 ohms' additional resistance was introduced, the value of Z was 40.5. The calculated value of A was 7000, and of β 3.45. In this case the values of Z as determined with the tissue only in the secondary circuit represent much more nearly the true relationships between the stimuli than do the values as determined with a large additional resistance in the circuit. In reality the stimulus applied in the first test

^{*} For the equations used in this calculation see p. 77.

was stronger than in the second, whereas, if reliance were placed upon the results given when the high additional resistance was in circuit, it would appear that the second stimulus was more than twice as strong as the first. The subjoined tabulation will serve to emphasize the error:

Z	(tissue only)	Z (70,000 ohms added)	β
First	6.6	16.8	4.I
Second	6.1	40.5	3.45
Ratio of 1st to 2d	1.08	0.41	1.10

In determining specific stimulation values by means of the expression $\beta = \frac{ZA}{R+A}$, particularly when the tissues stimulated have high resistances, errors in determining the value of A may easily vitiate the results. It will usually be found desirable to determine values of Z for at least three secondary resistances in addition to the tissue resistance itself. If the values of Z thus obtained are plotted against their respective resistances the curve which they yield reveals at once whether errors have been made in the determinations. The curve should be a straight line, cutting the ordinate for zero resistance at some point above the base line. Minor errors may be allowed for by drawing the curve to make them balance one another. This precaution is unnecessary when tissues of low resistance are studied, since with them small errors in determining A are less significant.

These are among the less obvious sources of error in

quantitative work, and are therefore discussed here. The more apparent ones need not be mentioned, since they are sure to suggest themselves to any user of the method here presented.

In the use of this quantitative method, as in most procedures involving numerous factors, a technique, which seems at the outset highly complicated, becomes with practice easy to carry out. Its inclusion as part of the experimental routine of the working physiologist is therefore justified. To facilitate such inclusion is the purpose of this manual.



INDEX

Ammeter, use of, 24. shunt for, 24.

du Bois Reymond inductorium, 3.
Break induced currents, 7.
Break shocks, course of, 32.
equation for, 35, 60.

Calibration of inductorium, apparatus required for, 23.

for break shocks, 55.

in region of iron core, 58.

Cathode, method of determining, 107.

Circuit, primary, make and break of, 60.

variables concerned in, 13. variations in break of, 60. variations in make of, 61.

secondary, variables concerned in, 13.

Coil, secondary, effect of position of on strength of shock, 7, 13, 15. Core, iron, correction for magnetization of, 46.

effects of on stimulation strengths, 43.

in critical region, 47. magnetization of, 43.

Current density, importance of, 76.

extra, 10.

induced, 5.

direction and intensity of, 5. method of varying, 7. sources of variation in, 13.

primary, adjustment of, 25.

measurement of, 24.

voltage, relation of to make stimuli, 97.

II4 INDEX

Density of current, importance of, 76.

Edelmann method of measuring induction shocks, 20. Electrodynamometer of Hoorweg-Giltay, 21. Electrode contacts, effect of on strength of shocks, 13, 76. Electrodes, needle, 27.

Sherrington, 27.

Extra current, 10.

Faradimeter of Edelmann, 20.

Fick-Meyer method of measuring induction shocks, 15.

v. Fleischl method of measuring induction shocks, 18.

application of, to calibration, 56.

Force, lines of, 5.

Galvanometer, ballistic, 26.

Hoorweg-Giltay method of measuring induction shocks, 21.

Induced current, direction and intensity of, 5.
form of, 8.
break, course of, 32.
make and break, 7.
measurement of, historical, 14.
method of varying, 7.
sources of variation in, 13.

Inductance, 8.

of secondary coil, 34. determination of, 50. equation for, 53.

Induction, discovery of, 2.

mutual, 34.

determination of, 38. relation of to calibration, 36.

Induction coil, standard, for use in calibration, 26.

structure of, 3.

Induction shocks, apparatus for quantitative use of, 30. break, course of, 32.

Induction shocks, break, equation for, 35.

comparison of make and break, 102.

make, measurement of, 94.

equation for, 99.

measurement of historical, 14.

Edelmann method, 20.
v. Fleischl method, 18.
Hoorweg-Giltay method, 21.
Kronecker method, 16.
Meyer-Fick method, 15.
Pflüger method, 14.
Wertheim-Salomonson method.

18.

sources of variation in, 13. stimulate at cathode, 72, 107.

Inductorium, du Bois Reymond type, 3.

principle of, 4.

calibration of, apparatus required, 23.

procedure, 28.

for break shocks, 55.

for make shocks, 94.

in region of iron core, 58.

"standard," 23, 88.

Berlin standard, 88.

shortcomings of, 92.

structure of, 3.

effect of on strength of shock, 13. relation to determination of specific stimulus, 78.

Iron core, effect of on strength of shock, 13, 43.

in critical region, 47.

magnetization of, 43.

correction for, 46.

Key, automatic, necessity for, 61.

knife-blade, construction of, 63.

advantages of, 64, 67, 70.

operating device for, 65.

116 INDEX

Key, knife-blade, short-circuiting device for, 67.
make and break, essentials of, 62.
Kronecker method of measuring induction shocks, 16.

Magnetization of core, correction for, 46.

Make induced currents, 7.

shocks, equation for, 99.

measurement of, 94. constant, determination of, 104.

Meyer-Fick method of measuring induction shocks, 15.

Pflüger method of measuring induction shocks, 14. Primary circuit, make and break of, 60.

variables concerned in, 13. variations in break of, 60. in make of, 61.

current, adjustment of, 25.

measurement of, 24.

relation of to strength of shock, 13.

voltage, relation of to make stimuli, 97.

Resistance of tissue, apparatus for measuring, 26.

determination of, 72.

effect of on strength of shock, 13, 73.

relation of to secondary resistance, 71.

Secondary circuit, variables concerned in, 13. Shocks, induction, sources of variation in, 13.

comparison of make and break, 102.

break, course of, 32.

equation for, 35, 60.

make, form of, 8.

equation for, 99.

determination of constant for, 104.

Short-circuiting device for knife-blade key, 67.

Shunt for ammeter, 24.

Specific stimuli, precautions necessary in obtaining, 110. Stimuli, faradic, historical, 14.

INDEX 117

Stimulus, actual, equation for, 76.

precautions necessary in obtaining, 110.

when not essential, 80.

Tissue resistance, apparatus for measuring, 26.

determination of, 72.

effect of, on strength of stimulus, 13, 73.

importance of, 21.

relation of to entire resistance, 71.

Voltage of primary current, relation of to make stimuli, 97.

Wertheim-Salomonson method of measuring induction shocks, 18.







SHORT-TITLE CATALOGUE

OF THE

PUBLICATIONS

OF

JOHN WILEY & SONS

NEW YORK

LONDON: CHAPMAN & HALL, LIMITED

ARRANGED UNDER SUBJECTS

Descriptive circulars sent on application. Books marked with an asterisk (*) are sold at net prices only. All books are bound in cloth unless otherwise stated.

AGRICULTURE-HORTICULTURE-FORESTRY.

MONICODIONE MONICODIONE TONDOINT.		
Armsby's Principles of Animal Nutrition8vo,	84	00
* Bowman's Forest Physiography8vo,		00
Budd and Hansen's American Horticultural Manual:		
Part I. Propagation, Culture, and Improvement	1	50
Part II. Systematic Pomology12mo,	1	50
Elliott's Engineering for Land Drainage12mo,	2	00
Practical Farm Drainage. (Second Edition, Rewritten.)12mo,	1	50
Fuller's Water Supplies for the Farm. (In Press.)		
Graves's Forest Mensuration8vo,		00
* Principles of Handling WoodlandsLarge 12mo,	-	50
Green's Principles of American Forestry	- 50	50
Grotenfelt's Principles of Modern Dairy Practice. (Woll.)12mo,	2	00
Hawley and Hawes's Practical Forestry for New England. (In Press.)	4	00
* Herrick's Denatured or Industrial Alcohol	-	50
* McKay and Larsen's Principles and Practice of Butter-making 8vo,		50
Maynard's Landscape Gardening as Applied to Home Decoration12mo,		50
Record's Identification of the Economic Woods of the United States. (In Press.		00
Sanderson's Insects Injurious to Staple Crops		50
* Insect Pests of Farm, Garden, and Orchard Large 12mo.	-	00
* Schwarz's Longleaf Pine in Virgin Forest		25
* Solotaroff's Field Book for Street-tree Mapping	0	75
In lots of one dozen	8	00
* Shade Trees in Towns and Cities8vo,		00
Stockbridge's Rocks and Soils8vo,		50
Winton's Microscopy of Vegetable Foods8vo,		50
Woll's Handbook for Farmers and Dairymen16mo,	1	50
ARCHITECTURE.		
* Atkinson's Orientation of Buildings or Planning for Sunlight 8vo,	2	00
Baldwin's Steam Heating for Buildings		50
Berg's Buildings and Structures of American Railroads4to,		00

Birkmire's Architectural Iron and Steel		50 00
Planning and Construction of High Office Buildings		50
Briggs's Modern American School Buildings8vo,		00
Byrne's Inspection of Materials and Workmanship Employed in Construction.		00
Carpenter's Heating and Ventilating of Buildings8vo,		00
* Corthell's Allowable Pressure on Deep Foundations	1	25
* Eckel's Building Stones and Clays		00 50
Fire Prevention and Fire Protection. (In Press.)	3	30
Fireproofing of Steel Buildings		50
vised and Enlarged.)	3	50
Sanitation of Public Buildings		50
Theatre Fires and Panics	1	50
8vo.	4	00
Johnson's Statics by Algebraic and Graphic Methods8vo.	2	00
Kellaway's How to Lay Out Suburban Home Grounds	5	
Merrill's Stones for Building and Decoration8vo,	5	00
Monckton's Stair-building	4	
Peabody's Naval Architecture8vc,	5 7	
Rice's Concrete-block Manufacture8vo,	2	00
Richey's Handbook for Superintendents of Construction 16mo, mor. Building Foreman's Pocket Book and Ready Reference 16mo, mor.	5	
* Building Mechanics' Ready Reference Series:		00
* Carpenters' and Woodworkers' Edition16mo, mor. * Cement Workers' and Plasterers' Edition16mo, mor.	1 .	
* Plumbers', Steam-Fitters', and Tinners' Edition16mo, mor.	1	_
* Stone- and Brick-masons' Edition16mo, mor.	1 .	
Sabin's House Painting	1 1	
Snow's Principal Species of Wood8vo,	3 .	50
Wait's Engineering and Architectural Jurisprudence8vo, Sheep.	6	
Law of Contracts8vo,	3 (
Law of Operations Preliminary to Construction in Engineering and Architecture	5 (00
Sheep,	5	20
Wilson's Air Conditioning	1 :	50
Worcester and Atkinson's Small Hospitals, Establishment and Maintenance, Suggestions for Hospital Architecture, with Plans for a Small		
Hospital12mo,	1 :	25
ARMY AND NAVY.		
Bernadou's Smokeless Powder, Nitro-cellulose, and the Theory of the Cellu-		
lose Molecule	2 1	
Screw Propellers and Marine Propulsion8vo,	3 (00
* Cloke's Enlisted Specialists' Examiner	2 (
Craig's Azimuth4to,	3 8	
Crehore and Squier's Polarizing Photo-chronograph8vo,	3 (
* Davis's Elements of Law	2 5	
* Dudley's Military Law and the Procedure of Courts-martialLarge 12mo,	2 1	50
Durand's Resistance and Propulsion of Ships8vo. * Dyer's Handbook of Light Artillery	5 (
Ly or a range of the bar and the control of the con	1	1757

Eissler's Modern High Explosives8vo	\$4 00)
* Fiebeger's Text-book on Field FortificationLarge 12mo,	2 00)
Hamilton and Bond's The Gunner's Catechism18mo,	1 00)
* Hoff's Elementary Naval Tactics	1 50	
Ingalls's Handbook of Problems in Direct Fire8vo,	4 00	
* Interior Ballistics	3 00	
* Lissak's Ordnance and Gunnery8vo,	6 00	
* Ludlow's Logarithmic and Trigonometric Tables	1 00	
* Lyons's Treatise on Electromagnetic Phenomena. Vols. I. and II8vo,each, * Mahan's Permanent Fortifications. (Mercur.)8vo, half mor.	6 00	
Manual for Courts-martial	1 50	
* Mercur's Attack of Fortified Places	2 00	
* Elements of the Art of War8vo,	4 00	
Nixon's Adjutants' Manual	1 00	
Peabody's Naval Architecture8vo,	7 50	
* Phelps's Practical Marine Surveying8vo,	2 50	
Putnam's Nautical Charts8vo,	2 00)
Rust's Ex-meridian Altitude, Azimuth and Star-Finding Tables8vo,	5 00)
* Selkirk's Catechism of Manual of Guard Duty	0 50)
Sharpe's Art of Subsisting Armies in War18mo, mor.	1 50	
* Taylor's Speed and Power of Ships. 2 vols. Text 8vo, plates oblong 4to,	7 50)
* Tupes and Poole's Manual of Bayonet Exercises and Musketry Fencing.	2 22	
* Weaver's Military Explosives	0 50	
* Weaver's Military Explosives	3 00	
* Woodhull's Military Hygiene for Officers of the LineLarge 12mo,	1 50	,
ASSAYING.		
Betts's Lead Refining by Electrolysis8vo,	4 00)
*Butler's Handbook of Blowpipe Analysis	0 75	
Fletcher's Practical Instructions in Quantitative Assaying with the Blowpipe.		
16mo, mor.	1 50)
Furman and Pardoe's Manual of Practical Assaying8vo,	3 00)
Lodge's Notes on Assaying and Metallurgical Laboratory Experiments8vo,	3 00)
Low's Technical Methods of Ore Analysis8vo,	3 00	
Miller's Cyanide Process	1 00	
Manual of Assaying	1 00	
Minet's Production of Aluminum and its Industrial Use. (Waldo.)12mo,	2 50	
Ricketts and Miller's Notes on Assaying	3 00	
Robine and Lenglen's Cyanide Industry. (Le Clerc.)8vo,	4 00	
* Seamon's Manual for Assayers and ChemistsLarge 12mo, Ulke's Modern Electrolytic Copper Refining8vo,	2 50	
Wilson's Chlorination Process	1 50	
Cyanide Processes	1 50	
Cyamide 110ccsscs	1 00	
ASTRONOMY.		
Comstock's Field Astronomy for Engineers8vo,	2 50	
Craig's Azimuth4to,	3 50	
Crandall's Text-book on Geodesy and Least Squares8vo,	3 00	
Doolittle's Treatise on Practical Astronomy8vo,	4 00	
Hayford's Text-book of Geodetic Astronomy8vo,	3 00	
Hosmer's Azimuth	1 00	
* Text-book on Practical Astronomy	2 00 2 50	
Merriman's Elements of Precise Surveying and Geodesy	3 00	
Rust's Ex-meridian Altitude, Azimuth and Star-Finding Tables8vo,	5 00	
* White's Elements of Theoretical and Descriptive Astronomy12mo,	2 00	
The state of the s		
CHEMISTRY.		
* Abderhalden's Physiological Chemistry in Thirty Lectures. (Hall and	5 00	
Defren.)	1 25	
Alexeyeff's General Principles of Organic Syntheses. (Matthews.)8vo,	3 00	
and a delicate a time place of organic of interests, (butterions, /11/11/10/0)	000	

	Allon's Tobles for Iron Applicate	00	00
	Allen's Tables for Iron Analysis	33	00
	Armsby's Principles of Animal Nutrition		
	Arnold's Compendium of Chemistry. (Mandel.)Large 12mo,	3	50
	Association of State and National Food and Dairy Departments, Hartford		
	Meeting, 19068vo,	3	00
	Jamestown Meeting, 19078vo,	3	00
	Austen's Notes for Chemical Students	1	50
	Bernadou's Smokeless PowderNitro-cellulose, and Theory of the Cellulose		
	Molecule	2	50
	* Biltz's Introduction to Inorganic Chemistry. (Hall and Phelan.)12mo,		25
10	Laboratory Methods of Inorganic Chemistry. (Hall and Blanchard.)	-	20
	8vo.	2	00
	* Bingham and White's Laboratory Manual of Inorganic Chemistry 12mo.		00
	* Blanchard's Synthetic Inorganic Chemistry		00
	* Bottler's German and American Varnish Making. (Sabin.) Large 12mo,	3	50
	Browne's Handbook of Sugar Analysis. (In Press.)		
	* Browning's Introduction to the Rarer Elements8vo,	1	50
	* Butler's Handbook of Blowpipe Analysis	0	75
	* Claassen's Beet-sugar Manufacture. (Hall and Rolfe.)8vo,		00
	Classen's Quantitative Chemical Analysis by Electrolysis. (Boltwood.).8vo,		00
	Cohn's Indicators and Test-papers		00
	Tests and Reagents		00
		0	00
	Cohnheim's Functions of Enzymes and Ferments. (In Press.)	-	-
	* Danneel's Electrochemistry. (Merriam.)		25
	Dannerth's Methods of Textile Chemistry12mo,		00
	Duhem's Thermodynamics and Chemistry. (Burgess.)8vo,		00
	Effront's Enzymes and their Applications. (Prescott.)8vo,	3	00
	Eissler's Modern High Explosives8vo,	4	00
	* Fischer's Oedema8vo,	2	00
	* Physiology of Alimentation Large 12mo,		00
	Fletcher's Practical Instructions in Quantitative Assaying with the Blowpipe.	-	00
		1	=0
	Fowler's Sewage Works Analyses	1	50
-	Fowler's Sewage Works Analyses	2	00
	Fresenius s Manual of Qualitative Chemical Analysis. (Wells.)8vo,	5	00
	Manual of Qualitative Chemical Analysis. Part I. Descriptive. (Wells.)8vo		
	Quantitative Chemical Analysis. (Cohn.) 2 vols8vc,	12	50
	When Sold Separately, Vol. I, \$6. Vol. II, \$8.		
1	Fuertes's Water and Public Health12mo,	1	50
	Furman and Pardoe's Manual of Practical Assaying8vo,	3	00
	* Getman's Exercises in Physical Chemistry		00
	Gill's Gas and Fuel Analysis for Engineers		25
	Gooch's Summary of Methods in Chemical Analysis. (In Press.)	-	-0
	Gooch and Browning's Outlines of Qualitative Chemical Analysis.		
			0=
	Large 12mo,		25
	Grotenfelt's Principles of Modern Dairy Practice. (Woll.)12mo,		00
	Groth's Introduction to Chemical Crystallography (Marshall) 12mo,		25
	* Hammarsten's Text-book of Physiological Chemistry. (Mandel.)8vo,		00
	Hanausek's Microscopy of Technical Products. (Winton.)8vo,		00
	* Haskins and Macleod's Organic Chemistry	2	00
-	* Herrick's Denatured or Industrial Alcohol8vo,	4	00
	Hinds's Inorganic Chemistry8vo,	3	00
	* Laboratory Manual for Students.,		00
-	* Holleman's Laboratory Manual of Organic Chemistry for Beginners.	-	
	(Walker.)	1	00
	Text-book of Inorganic Chemistry. (Cooper.)8vo,		50
	Text-book of Organic Chemistry. (Walker and Mott.)8vo,	2	50
	Holley's Analysis of Paint and Varnish Products. (In Press.)		-
	* Lead and Zinc PigmentsLarge 12mo,		00
	Hopkins's Oil-chemists' Handbook8vo		00
	Jackson's Directions for Laboratory Work in Physiological Chemistry 8vo,	1	25
	Johnson's Rapid Methods for the Chemical Analysis of Special Steels, Steel-		
	making Alloys and GraphiteLarge 12mo,	3	00
1	Landauer's Spectrum Analysis. (Tingle.)8vo,	3	00
	Lassar-Cohn's Application of Some General Reactions to Investigations in	The same	
	Organic Chemistry. (Tingle.)	1	00
	Leach's Inspection and Analysis of Food with Special Reference to State	WE!	
	Control	7	50
			00

		0.00
Löb's Electrochemistry of Organic Compounds. (Lorenz.)8vo,		
Lodge's Notes on Assaying and Metallurgical Laboratory Experiments8vo,	3 (00
Low's Technical Method of Ore Analysis8vo,	3 (00
Lowe's Paint for Steel Structures12mo,	1 (00
Lunge's Techno-chemical Analysis. (Cohn.)	1 (
Lunge's Techno-chemical Analysis. (Cont.)	1	
* McKay and Larsen's Principles and Practice of Butter-making 8vo,		
Maire's Modern Pigments and their Vehicles12mo,	2 (
Mandel's Handbook for Bio-chemical Laboratory	1 !	50
* Martin's Laboratory Guide to Qualitative Analysis with the Blowpipe		
12mo,	0 6	0.8
	1 :	
Mason's Examination of Water. (Chemical and Bacteriological.)12mo,	1 .	20
Water-supply. (Considered Principally from a Sanitary Standpoint.)		
8vo,	4 (00
* Mathewson's First Principles of Chemical Theory8vo,	1 (00
Matthews's Laboratory Manual of Dyeing and Textile Chemistry 8vo,	3 .	
Matthews & Laboratory Manual of Dynamic and Textue Chemistry	4 (
Textile Fibres. 2d Edition, Rewritten8vo.	4	00
* Meyer's Determination of Radicles in Carbon Compounds. (Tingle.)		
Third Edition12mo,	1 :	25
Miller's Cyanide Process12mo,	1 (00
Manual of Assaying12mo,	1 (00
Minet's Production of Aluminum and its Industrial Use. (Waldo.)12mo,	2	
Minet's Production of Authintum and its industrial of the Wards (Nation)12mo,	1	
* Mittelstaedt's Technical Calculations for Sugar Works. (Bourbakis.) 12mo,		
Mixter's Elementary Text-book of Chemistry12mo,	1 .	
Morgan's Elements of Physical Chemistry12mo,	3 (00
* Physical Chemistry for Electrical Engineers	1 .	50
* Moore's Experiments in Organic Chemistry	0	
	1	
* Outlines of Organic Chemistry12mo,		
Morse's Calculations used in Cane-sugar Factories16mo, mor.	1 .	
* Muir's History of Chemical Theories and Laws8vo,	4	00
Mulliken's General Method for the Identification of Pure Organic Compounds.		
Vol. I. Compounds of Carbon with Hydrogen and Oxygen. Large 8vo,	5	00
Vol. 1. Compounds of Carbon vol. (In Proposition)		
Vol. II. Nitrogenous Compounds. (In Preparation.)	-	00
Vol. III. The Commercial DyestuffsLarge 8vo,	5	
* Nelson's Analysis of Drugs and Medicines	5	
Ostwald's Conversations on Chemistry. Part One. (Ramsey.)12mo,	1	50
" Part Two (Turnbull) 12mo.	2	00
* Introduction to Chemistry. (Hall and Williams.)Large 12mo,	1	
Introduction to Chemistry. (Italia and Windams)		00
Owen and Standage's Dyeing and Cleaning of Textile Fabrics12mo,		
* Palmer's Practical Test Book of Chemistry	1	00
* Pauli's Physical Chemistry in the Service of Medicine. (Fischer.)12mo,	1	25
Penfield's Tables of Minerals, Including the Use of Minerals and Statistics		
of Domestic Production8vo,	1	00
Pictet's Alkaloids and their Chemical Constitution. (Biddle.)8vo,	5	00
Picter's Aikaloids and their Chemical Constitution.	-	
	2	
Poole's Calorific Power of Fuels	3	00
Prescott and Winslow's Elements of Water Bacteriology, with Special Refer-		
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1	50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1	50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1	50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25	50 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2	50 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3	50 00 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4	50 00 00 00 00 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1	50 00 00 00 00 00 25
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4	50 00 00 00 00 00 25 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4	50 00 00 00 00 00 25
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2	50 00 00 00 00 00 25 00 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1	50 00 00 00 00 25 00 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3	50 00 00 00 00 25 00 00 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3	50 00 00 00 00 25 00 00 00 00 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2	50 00 00 00 00 25 00 00 00 00 00 50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1	50 00 00 00 00 25 00 00 00 00 00 50 50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5	50 00 00 00 00 25 00 00 00 00 00 50 50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5	50 00 00 00 00 25 00 00 00 00 00 50 50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5 1	50 00 00 00 00 25 00 00 00 00 50 50 00 25
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5 1 2	50 00 00 00 00 25 00 00 00 00 50 50 00 25 50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5 1 2 2	50 00 00 00 00 25 00 00 00 50 50 50 25 50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5 1 2 3	50 00 00 00 00 25 00 00 00 50 50 50 50 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5 1 2 2 3 3 3 3 3 3 3 3 3 3 3 3 3 3 3 3 3	50 00 00 00 00 25 00 00 00 50 50 50 00 25 50 00 00
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5 1 2 2 3 3 2 2 2 3 2 2 2 2 2 2 3 3 2	50 00 00 00 00 25 00 00 00 50 50 50 00 00 00 50 50
Prescott and Winslow's Elements of Water Bacteriology, with Special Reference to Sanitary Water Analysis	1 25 2 3 4 1 4 2 1 3 3 2 1 5 1 2 2 3 3 2 2 2 3 2 2 2 2 2 2 3 3 2	50 00 00 00 00 25 00 00 00 50 50 50 00 25 50 00 00

* Tillman's Descriptive General Chemistry8vo,	
* Elementary Lessons in Heat8vo,	1 50
Treadwell's Qualitative Analysis. (Hall.)8vo,	3 00 4 00
Quantitative Analysis, (Hall.)8vo, Turneaure and Russell's Public Water-supples8vo,	5 00
Van Deventer's Physical Chemistry for Beginners. (Boltwood.)12mo,	1 50
Venable's Methods and Devices for Bacterial Treatment of Sewage 8vo,	3 00
Ward and Whipple's Freshwater Biology. (In Press.)	
Ware's Beet-sugar Manufacture and Refining. Vol. I	4 00
" " Vol. II8vo,	5 00
Washington's Manual of the Chemical Analysis of Rocks8vo,	2 00 3 00
* Weaver's Military Explosives	1 50
Short Course in Inorganic Qualitative Chemical Analysis for Engineering	- 00
Students12mo,	1 50
Text-book of Chemical Arithmetic	1 25
Whipple's Microscopy of Drinking-water8vo,	3 50
Wilson's Chlorination Process	1 50 1 50
Winton's Microscopy of Vegetable Foods8vo,	7 50
Zsigmondy's Colloids and the Ultramicroscope. (Alexander.). Large 12mo,	3 00
CIVIL ENGINEERING.	
BRIDGES AND ROOFS. HYDRAULICS. MATERIALS OF ENGINE	FFP-
ING. RAILWAY ENGINEERING.	BER-
* American Civil Engineers' Pocket Book. (Mansfield Merriman, Editor-	
in-chief.)	5 00
Baker's Engineers' Surveying Instruments	3 00 0 25
Breed and Hosmer's Principles and Practice of Surveying. Vol. I. Elemen-	0 20
tary Surveying8vo,	3 00
Vol. II. Higher Surveying8vo,	2 50
* Burr's Ancient and Modern Engineering and the Isthmian Canal8vo,	3 50
Comstock's Field Astronomy for Engineers8vo,	2 50
* Corthell's Allowable Pressure on Deep Foundations	1 25 3 00
Davis's Elevation and Stadia Tables8vo,	1 00
* Eckel's Building Stones and Clays 8vo,	3 00
Elliott's Engineering for Land Drainage	2 00
* Fiebeger's Treatise on Civil Engineering8vo,	5 00
Flemer's Phototopographic Methods and Instruments8vo,	5 00
Folwell's Sewerage. (Designing and Maintenance.)	3 00 3 50
French and Ives's Stereotomy	2 50
Gilbert, Wightman, and Saunders's Subways and Tunnels of New York.	
(In Press.)	
* Hauch and Rice's Tables of Quantities for Preliminary Estimates 12mo,	1 25
Hayford's Text-book of Geodetic Astronomy8vo, Hering's Ready Reference Tables (Conversion Factors.)16mo, mor.	3 00 2 50
Hosmer's Azimuth	1 00
* Text-book on Practical Astronomy8vo,	2 00
Howe's Retaining Walls for Earth12mo,	1 25
* Ives's Adjustments of the Engineer's Transit and Level 16mo, bds.	0 25
Ives and Hilts's Problems in Surveying, Railroad Surveying and Geod-	1 50
esy	1 50 3 50
Johnson's (L. J.) Statics by Algebraic and Graphic Methods8vo,	2 00
* Kinnicutt, Winslow and Pratt's Sewage Disposal8vo,	3 00
* Mahan's Descriptive Geometry8vo,.	1 50
Merriman's Elements of Precise Surveying and Geodesy8vo,	2 50
Merriman and Brooks's Handbook for Surveyors16mo, mor.	2 00
Nugent's Plane Surveying	3 50
Sewer Design	2 00
THE RESIDENCE OF THE PROPERTY	

Ogden and Cleveland's Practical Methods of Sewage Disposal for Resi-		
dences, Hotels, and Institutions. (In Press.) Parsons's Disposal of Municipal Refuse8vo.	20	00
Patton's Treatise on Civil Engineering8vo, half leather.	7	50
Reed's Topographical Drawing and Sketching4to,	5	00
Riemer's Shaft-sinking under Difficult Conditions. (Corning and Peele.).8vo. Siebert and Biggin's Modern Stone-cutting and Masonry8vo.	3	00
Smith's Manual of Topographical Drawing. (McMillan.)		50 50
Soper's Air and Ventilation of Subways		50
* Tracy's Exercises in Surveying		00
Tracy's Plane Surveying		00
Methods and Devices for Bacterial Treatment of Sewage8vo,		00
Wait's Engineering and Architectural Jurisprudence8vo,		00
Law of Contracts		50
Law of Operations Preliminary to Construction in Engineering and	3	00
Architecture	5	00
Chan		50
Warren's Stereotomy—Problems in Stone-cutting	2	50
	1	00
* Enlarged Edition, Including Tables		50
Webb's Problems in the Use and Adjustment of Engineering Instruments.		
Wilson's Topographic Surveying8vo,		25
	0	50
BRIDGES AND ROOFS.		
Boller's Practical Treatise on the Construction of Iron Highway Bridges8vo,		00
* Thames River BridgeOblong paper, Burr and Falk's Design and Construction of Metallic Bridges8vo,		00
Influence Lines for Bridge and Roof Computations8vo,		00
Du Bois's Mechanics of Engineering. Vol. II	10	
Foster's Treatise on Wooden Trestle Bridges4to,		00
Fowler's Ordinary Foundations		50 50
Bridge Trusses8vo,		50
Roof Trusses8vo,	1.	25
Grimm's Secondary Stresses in Bridge Trusses	2	
Howe's Design of Simple Roof-trusses in Wood and Steel8vo.	3 2	
Symmetrical Masonry Arches8vo,	2	
Treatise on Arches8vo,	4	
* Hudson's Deflections and Statically Indeterminate Stresses Small 4to,	3	
* Plate Girder Design	2	
Johnson, Bryan and Turneaure's Theory and Practice in the Designing of		
Modern Framed StructuresSmall 4to, * Johnson, Bryan and Turneaure's Theory and Practice in the Designing of	10 (00
Modern Framed Structures. New Edition. Part I8vo.	3 (00
* Part II. New Edition8vo.	4 (
Merriman and Jacoby's Text-book on Roofs and Bridges:	-	
Part I. Stresses in Simple Trusses	2 1	
Part III. Bridge Design	2	
Part IV. Higher Structures8vo,	2 4	
Ricker's Design and Construction of Roofs. (In Press.) Sondericker's Graphic Statics, with Applications to Trusses, Beams, and		
Arches	2 (
* Specifications for Steel Bridges	2 (50
Waddell and Harrington's Bridge Engineering. (In Preparation.)		-
HYDRAULICS.		
Barnes's Ice Formation	3 (00
Bazin's Experiments upon the Contraction of the Liquid Vein Issuing from		
an Orifice. (Trautwine.)8vo,	2 0	00

Bovey's Treatise on Hydraulics	\$5 0	00
Oblong 4to, paper,	1 5	0
Hydraulic Motors	2 0	00
Mechanics of Fluids (Being Part IV of Mechanics of Engineering) 8vo,	3 0	
Coffin's Graphical Solution of Hydraulic Problems16mo, mor.	2 5	
Flather's Dynamometers, and the Measurement of Power12mo,	3 0	
Folwell's Water-supply Engineering8vo,	4 0	
Frizell's Water-power	5 0	
Water-filtration Works	1 5 2 5	
Ganguillet and Kutter's General Formula for the Uniform Flow of Water in	2 0	0
Rivers and Other Channels. (Hering and Trautwine.)8vo,	4 0	00
Hazen's Clean Water and How to Get ItLarge 12mo,	1 5	
Filtration of Public Water-supplies8vo,	3 0	
Hazelhurst's Towers and Tanks for Water-works8vo,	2 5	
Herschel's 115 Experiments on the Carrying Capacity of Large, Riveted, Metal		
Conduits8vo,	2 0	
Hoyt and Grover's River Discharge8vo,	2 0	0
Hubbard and Kiersted's Water-works Management and Maintenance.		-
*I1-' Development of District Of Williams Byo,	4 0	0
*Lyndon's Development and Electrical Distribution of Water Power.		^
Mason's Water-supply. (Considered Principally from a Sanitary Stand-	3 0	U
point.)8vo,	4 0	0
* Merriman's Treatise on Hydraulics. 9th Edition, Rewritten8vo.	4 0	
* Molitor's Hydraulics of Rivers, Weirs and Sluices8vo,	2 0	
* Morrison and Brodie's High Masonry Dam Design8vo,	1 5	
* Richards's Laboratory Notes on Industrial Water Analysis8vo,	5	
Schuyler's Reservoirs for Irrigation, Water-power, and Domestic Water-		
supply. Second Edition, Revised and EnlargedLarge 8vo,	6 0	0
* Thomas and Watt's Improvement of Rivers4to,	6 0	
Turneaure and Russell's Public Water-supplies8vo,	5 0	
* Wegmann's Design and Construction of Dams. 6th Ed., enlarged4to,	6 0	
	10 0	
Whipple's Value of Pure WaterLarge 12mo, Williams and Hazen's Hydraulic Tables8vo,	1 5	
Wilson's Irrigation Engineering8vo,	4 0	
Wood's Turbines8vo.	2 5	
WIMPRILLS OF THE STATE OF THE S		
MATERIALS OF ENGINEERING.		
Baker's Roads and Pavements8vo,	5 00	0
Treatise on Masonry Construction8vo,	5 00	
Black's United States Public WorksOblong 4to,	5 00	0
* Blanchard and Drowne's Highway Engineering, as Presented at the		
Second International Road Congress, Brussels, 19108vo,	2 00)
Bleininger's Manufacture of Hydraulic Cement. (In Preparation.)		
* Bottler's German and American Varnish Making. (Sabin.). Large 12mo.	3 50	
Burr's Elasticity and Resistance of the Materials of Engineering8vo, Byrne's Highway Construction8vo,	7 50	
	7 50	
Inspection of the Materials and Workmanship Employed in Construction	7 50 5 00	,
Inspection of the Materials and Workmanship Employed in Construction.	5 00	
Inspection of the Materials and Workmanship Employed in Construction. 16mo,	3 00)
Inspection of the Materials and Workmanship Employed in Construction.	5 00)
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. 8vo,	3 00)
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering	5 00 3 00 6 00 4 50)
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. No. Du Bois's Mechanics of Engineering. Vol. I. Kinematics, Statics, Kinetics. Small 4to,	5 00 3 00 6 00)
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering	5 00 3 00 6 00 4 50 7 50	
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. Nechanics of Engineering. Vol. I. Kinematics, Statics, Kinetics. Vol. II. The Stresses in Framed Structures, Strength of Materials and Theory of Flexures. Small 4to, 1	5 00 3 00 6 00 4 50 7 50 10 00	
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. No. Du Bois's Mechanics of Engineering. Vol. I. Kinematics, Statics, Kinetics. Vol. II. The Stresses in Framed Structures, Strength of Materials and Theory of Flexures. Small 4to, 1 * Eckel's Building Stones and Clays.	5 00 3 00 6 00 4 50 7 50 0 00 3 00	
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. No. Du Bois's Mechanics of Engineering. Vol. I. Kinematics, Statics, Kinetics. Vol. II. The Stresses in Framed Structures, Strength of Materials and Theory of Flexures. Small 4to, 1 * Eckel's Building Stones and Clays. * Cements, Limes, and Plasters. Svo.	5 00 3 00 6 00 4 50 7 50 0 00 3 00 6 00	
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. No. Du Bois's Mechanics of Engineering. Vol. I. Kinematics, Statics, Kinetics. Vol. II. The Stresses in Framed Structures, Strength of Materials and Theory of Flexures. * Eckel's Building Stones and Clays. * Cements, Limes, and Plasters. Svo, Fowler's Ordinary Foundations.	5 00 3 00 6 00 4 50 7 50 0 00 3 00 6 00 3 50	
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. No. Du Bois's Mechanics of Engineering. Vol. I. Kinematics, Statics, Kinetics. Vol. II. The Stresses in Framed Structures, Strength of Materials and Theory of Flexures. * Eckel's Building Stones and Clays. * Cements, Limes, and Plasters. Svo, Fowler's Ordinary Foundations. Svo, * Greene's Structural Mechanics. Svo,	5 00 3 00 6 00 4 50 7 50 0 00 3 00 6 00	
Inspection of the Materials and Workmanship Employed in Construction. 16mo, Church's Mechanics of Engineering. Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering. No. Du Bois's Mechanics of Engineering. Vol. I. Kinematics, Statics, Kinetics. Vol. II. The Stresses in Framed Structures, Strength of Materials and Theory of Flexures. * Eckel's Building Stones and Clays. * Cements, Limes, and Plasters. Svo, Fowler's Ordinary Foundations.	5 00 3 00 6 00 4 50 7 50 0 00 3 00 6 00 3 50	

* Hubbard's Dust Preventives and Road Binders	\$3 00
Steel-making Alloys and GraphiteLarge 12mo,	3 00
Johnson's (J. B.) Materials of ConstructionLarge 8vo,	6 00
Keep's Cast Iron8vo,	2 50
Lanza's Applied Mechanics	7 50
Maire's Modern Pigments and their Vehicles	2 00
* Martin's Text Book on Mechanics. Vol. I. Statics	1 25
* Vol. II. Kinematics and Kinetics	1 50
* Vol. III. Mechanics of Materials	1 50
Maurer's Technical Mechanics8vo,	4 00
Merrill's Stones for Building and Decoration8vo,	5 00
Merriman's Mechanics of Materials	5 00
Metcalf's Steel. A Manual for Steel-users12mo,	2 00
Morrison's Highway Engineering8vo,	2 50
* Murdock's Strength of Materials12mo,	2 00
Patton's Practical Treatise on Foundations8vo,	5 00
Rice's Concrete Block Manufacture8vo,	2 00
Richardson's Modern Asphalt Pavement8vo,	3 00
Richey's Building Foreman's Pocket Book and Ready Reference. 16mo, mor.	5 00
* Cement Workers' and Plasterers' Edition (Building Mechanics' Ready Reference Series)	1 50
Handbook for Superintendents of Construction16mo, mor.	4 00
*Stone and Brick Masons' Edition (Building Mechanics' Ready	1 00
Reference Series)16mo, mor.	1 50
* Ries's Clays: Their Occurrence, Properties, and Uses8vo,	5 00
* Ries and Leighton's History of the Clay-working Industry of the United	
States8vo.	2 50
Sabin's Industrial and Artistic Technology of Paint and Varnish8vo,	3 00
* Smith's Strength of Material	1 25 3 50
Snow's Principal Species of Wood	2 00
Text-book on Roads and Pavements	2 00
* Taylor and Thompson's Concrete Costs	5 00
* Extracts on Reinforced Concrete Design 8vo,	2 00
Treatise on Concrete, Plain and Reinforced8vo,	5 00
Thurston's Materials of Engineering. In Three Parts8vo,	8 00
Part I. Non-metallic Materials of Engineering and Metallurgy8vo,	2 00 3 50
Part II. Iron and Steel	3 30
Constituents8vo,	2 50
Tillson's Street Pavements and Paving Materials8vo,	4 00
Turneaure and Maurer's Principles of Reinforced Concrete Construction.	
Second Edition, Revised and Enlarged8vo,	3 50
Waterbury's Cement Laboratory Manual	1 00
* Laboratory Manual for Testing Materials of Construction 12mo,	1 50
Wood's (De V.) Treatise on the Resistance of Materials, and an Appendix on the Preservation of Timber8vo,	2 00
Wood's (M. P.) Rustless Coatings: Corrosion and Electrolysis of Iron and	2 00
Steel8vo,	4 00
RAILWAY ENGINEERING.	
Andrews's Handbook for Street Railway Engineers3×5 inches, mor.	1 25
Berg's Buildings and Structures of American Railroads4to,	5 00
Brooks's Handbook of Street Railroad Location16mo, mor.	1 50
* Burt's Railway Station Service	2 00
Butts's Civil Engineer's Field-book16mo, mor.	2 50
. Crandall's Railway and Other Earthwork Tables	1 50
Crandall and Barnes's Railroad Surveying	2 00
* Crockett's Methods for Earthwork Computations	5 00
Fisher's Table of Cubic Yards	25
Godwin's Railroad Engineers' Field-book and Explorers' Guide. 16mo, mor.	2 50

Hudson's Tables for Calculating the Cubic Contents of Excavations and Em-		A SOL
bankments	\$1	00
Molitor and Beard's Manual for Resident Engineers16mo, mor.		50
Nagle's Field Manual for Railroad Engineers	-	00
* Orrock's Railroad Structures and Estimates8vo,		00
Philbrick's Field Manual for Engineers		00
Elements of Railroad Engineering8vo,	3	50
Railroad Engineer's Field Book. (In Preparation.) Roberts' Track Formulæ and Tables	3	00
Searles's Field Engineering	3	00
Railroad Spiral		50 50
Webb's Economics of Railroad ConstructionLarge 12mo,	2	50
Railroad Construction		00
Wilson's Elements of Railroad-Track and Construction12mo,		00
DRAWING		
Barr and Wood's Kinematics of Machinery8vo,		50
* Bartlett's Mechanical Drawing		00 50
* Bartlett and Johnson's Engineering Descriptive Geometry8vo,		50
Blessing and Darling's Descriptive Geometry. (In Press.) Elements of Drawing. (In Press.)		
Coolidge's Manual of Drawing8vo, paper,	1	00
Coolidge and Freeman's Elements of General Drafting for Mechanical EngineersOblong 4to,	9	50
Durley's Kinematics of Machines8vo,	4	00
Emch's Introduction to Projective Geometry and its Application8vo, Hill's Text-book on Shades and Shadows, and Perspective8vo,		50 00
Jamison's Advanced Mechanical Drawing8vo,	2	00
Elements of Mechanical Drawing8vo, Jones's Machine Design:	2	50
Part I. Kinematics of Machinery8vo,		50
Part II. Form, Strength, and Proportions of Parts		00
MacCord's Elements of Descriptive Geometry8vo,	3	00
Kinematics; or, Practical Mechanism		00
Velocity Diagrams8vo,	1	50
McLeod's Descriptive GeometryLarge 12mo, * Mahan's Descriptive Geometry and Stone-cutting8vo,		50 50
Industrial Drawing. (Thempson.)8vo,	3	50
Moyer's Descriptive Geometry	1700	00
* Reid's Mechanical Drawing. (Elementary and Advanced.)8vo,	2	00
Text-book of Mechanical Drawing and Elementary Machine Design8vo, Robinson's Principles of Mechanism8vo,		00
Schwamb and Merrill's Elements of Mechanism8vo,	3	00
Smith (A. W.) and Marx's Machine Design		00 50
* Titsworth's Elements of Mechanical DrawingOblong 8vo,		25
Tracy and North's Descriptive Geometry. (In Press.) Warren's Elements of Descriptive Geometry, Shadows, and Perspective. 8vo,	2	50
Elements of Machine Construction and Drawing8vo,	7	50
Elements of Plane and Solid Free-hand Geometrical Drawing12mo, General Problems of Shades and Shadows8vo,		00
Manual of Elementary Problems in the Linear Perspective of Forms and		
Shadow		00 50
Plane Problems in Elementary Geometry12mo,		25
Weisbach's Kinematics and Power of Transmission. (Hermann and Klein.)	5	00
Zalom, it it is it		

Wilson's (H. M.) Topographic Surveying	1 50 1 00 2 50
Woolf's Elementary Course in Descriptive GeometryLarge 8vo,	3 00
ELECTRICITY AND PHYSICS.	
* Abegg's Theory of Electrolytic Dissociation. (von Ende.)	1 25 1 25
ments12mo,	1 00
Anthony and Brackett's Text-book of Physics. (Magie.)Large 12mo, Benjamin's History of Electricity8vo,	3 00
Betts's Lead Refining and Electrolysis	4 00
Edition	4 00 3 00
* Collins's Manual of Wireless Telegraphy and Telephony	1 50 3 00
* Danneel's Electrochemistry. (Merriam.)	1 25
Dawson's "Engineering" and Electric Traction Pocket-book16mo, mor. Dolezalek's Theory of the Lead Accumulator (Storage Battery). (von Ende.)	5 00
Duhem's Thermodynamics and Chemistry. (Burgess.)8vo,	2 50 4 00
Flather's Dynamometers, and the Measurement of Power	3 00 1 50
* Getman's Introduction to Physical Science	2 50
* Hanchett's Alternating Currents	1 00 2 50
* Hobart and Ellis's High-speed Dynamo Electric Machinery8vo,	6 00
Holman's Precision of Measurements	2 00 0 75
* Hutchinson's High-Efficiency Electrical Illuminants and Illumination.	0 13
Large 12mo,	2 50 4 00
* Jones's Electric Ignition	3 50
* Vol. II	2 50 2 00
Landauer's Spectrum Analysis. (Tingle.)8vo,	3 00
Löb's Electrochemistry of Organic Compounds. (Lorenz.)	3 00
* Lyons's Treatise on Electromagnetic Phenomena. Vols, I. and II. 8vo, each,	6 00
* Michie's Elements of Wave Motion Relating to Sound and Light8vo, * Morgan's Physical Chemistry for Electrical Engineers12mo,	4 00
* Norris's Introduction to the Study of Electrical Engineering8vo, Norris and Dennison's Course of Problems on the Electrical Characteristics of	2 50
Circuits and Machines. (In Press.) * Parshall and Hobart's Electric Machine Design4to, half mor, Reagan's Locomotives: Simple, Compound, and Electric. New Edition.	12 50
Large 12mo,	
* Rosenberg's Electrical Engineering. (Haldane Gee—Kinzbrunner.)8vo, * Ryan's Design of Electrical Machinery:	
* Vol. I. Direct Current Dynamos	
(In Preparation.)	
Ryan, Norris, and Hoxie's Text Book of Electrical Machinery8vo, Schapper's Laboratory Guide for Students in Physical Chemistry12mo,	2 50
* Tillman's Elementary Lessons in Heat8vo,	1 50
* Timbie's Elements of ElectricityLarge 12mo, * Answers to Problems in Elements of Electricity12mo, Paper	2 00 0 25
Tory and Pitcher's Manual of Laboratory PhysicsLarge 12mo,	2 00
* Waters's Commercial Dynamo Design	2 00

LAW.

* Brennan's Hand-book of Useful Legal Information for Business Men.	
* Davis's Elements of Law	
* Davis's Elements of Law	2 50 7 00
* Dudley's Military Law and the Procedure of Courts-martial. Large 12mo,	2 50
Manual for Courts-martial16mo, mor.	1 50
Wait's Engineering and Architectural Jurisprudence8vo,	6 00
Law of Contracts	6 50
Law of Operations Preliminary to Construction in Engineering and	3 00
Architecture8vo,	5 00
Sheep,	5 50
MATHEMATICS.	
Baker's Elliptic Functions8vo,	1 50
Briggs's Elements of Plane Analytic Geometry. (Bôcher.)	1 00
* Buchanan's Plane and Spherical Trigonometry8vo,	1 00
Byerly's Harmonic Functions8vo,	1 00
Chandler's Elements of the Infinitesimal Calculus	2 00 2 50
Compton's Manual of Logarithmic Computations	1 50
* Dickson's College AlgebraLarge 12mo,	1 50
* Introduction to the Theory of Algebraic Equations Large 12mo,	1 25
Emch's Introduction to Projective Geometry and its Application8vo,	2 50
Fiske's Functions of a Complex Variable	1 00
Elements of Geometry8vo,	1 75
* Rational Geometry	1 50
Synthetic Projective Geometry8vo,	1 00
* Hancock's Lectures on the Theory of Elliptic Functions	5 00
* Johnson's (J. B.) Three-place Logarithmic Tables: Vest-pocket size, paper,	0 15
* 100 copies,	5 00
* Mounted on heavy cardboard, 8×10 inches, * 10 copies,	0 25 2 00
Johnson's (W. W.) Abridged Editions of Differential and Integral Calculus.	2 00
Large 12mo, 1 vol.	2 50
Curve Tracing in Cartesian Co-ordinates	1 00
Differential Equations	1 00
Elementary Treatise on the Integral CalculusLarge 12mo,	1 50
* Theoretical Mechanics	3 00
Theory of Errors and the Method of Least Squares	1 50
Treatise on Differential Calculus	3 00
Treatise on Ordinary and Partial Differential EquationsLarge 12mo,	3 50
Karapetoff's Engineering Applications of Higher Mathematics:	
* Part I. Problems on Machine Design Large 12mo,	0 75
Koch's Practical Mathematics. (In Press.) Laplace's Philosophical Essay on Probabilities. (Truscott and Emory.). 12mo,	2 00
* Le Messurier's Key to Professor W. W. Johnson's Differential Equations.	2 00
Small 8vo,	1 75
* Ludlow's Logarithmic and Trigonometric Tables 8vo, * Ludlow and Bass's Elements of Trigonometry and Logarithmic and Other	1 00
Tables8vo,	3 00
* Trigonometry and Tables published separately Each,	2 00
Macfarlane's Vector Analysis and Quaternions8vo,	1 00
McMahon's Hyperbolic Functions	1 00
Series	1 25
* Martin's Text Book on Mechanics. Vol. I. Statics	1 25
* Vol. II. Kinematics and Kinetics	1 50
* Vol. III. Mechanics of Materials12mo,	1 50

S. WoodwardOctavo, each	\$1 00
No. 1. History of Modern Mathematics, by David Eugene Smith.	
No. 2. Synthetic Projective Geometry, by George Bruce Halsted	
No. 3. Determinants, by Laenas Gifford Weld. No. 4. Hyper-	
bolic Functions, by James McMahon. No. 5. Harmonic Func-	
tions, by William E. Byerly. No. 6. Grassmann's Space Analysis,	
by Edward W. Hyde. No. 7. Probability and Theory of Errors,	
by Robert S. Woodward. No. 8. Vector Analysis and Quaternions,	
by Alexander Macfarlane. No. 9. Differential Equations, by	
William Woolsey Johnson. No. 10. The Solution of Equations,	
by Mansfield Merriman. No. 11. Functions of a Complex Variable,	
by Thomas S. Fiske. Maurer's Technical Mechanics8vo.	4 00
Merriman's Method of Least Squares	4 00 2 00
Solution of Equations8vo,	1 00
* Moritz's Elements of Plane Trigonometry8vo,	2 00
Rice and Johnson's Differential and Integral Calculus. 2 vols. in one.	2 00
Large 12mo.	1 50
Elementary Treatise on the Differential Calculus Large 12mo,	3 00
Smith's History of Modern Mathematics8vo,	1 00
* Veblen and Lennes's Introduction to the Real Infinitesimal Analysis of One	
Variable8vo,	2 00
* Waterbury's Vest Pocket Hand-book of Mathematics for Engineers.	
$2\frac{7}{8} \times 5\frac{3}{8}$ inches, mor.	1 00
* Enlarged Edition, Including Tablesmor.	1 50
Weld's Determinants8vo,	1 00
Wood's Elements of Co-ordinate Geometry8vo,	2 00
Woodward's Probability and Theory of Errors8vo,	1 00
MEGITINIAL PROFESSION	
MECHANICAL ENGINEERING.	
MATERIALS OF ENGINEERING, STEAM-ENGINES AND BOILE	RS.
Bacon's Forge Practice	1 50
Baldwin's Steam Heating for Buildings12mo,	
	2 50
Barr and Wood's Kinematics of Machinery8vo,	2 50
Barr and Wood's Kinematics of Machinery	2 50 3 00
Barr and Wood's Kinematics of Machinery	2 50 3 00 1 50
Barr and Wood's Kinematics of Machinery	2 50 3 00 1 50 1 50
Barr and Wood's Kinematics of Machinery	2 50 3 00 1 50 1 50 3 50
Barr and Wood's Kinematics of Machinery	2 50 3 00 1 50 1 50 3 50 4 00
Barr and Wood's Kinematics of Machinery	2 50 3 00 1 50 1 50 3 50 4 00 6 00
Barr and Wood's Kinematics of Machinery	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing 8vo, * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing 8vo, * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, * Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo, Coolidge's Manual of Drawing 8vo, paper,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00
Barr and Wood's Kinematics of Machinery	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 00
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing 8vo, * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, * Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo, Compton and De Groodt's Speed Lathe 12mo, Coolidge's Manual of Drawing 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers 0blong 4to,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing 8vo, * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, * Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo, Compton and De Groodt's Speed Lathe 12mo, Coolidge's Manual of Drawing 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers 0blong 4to, Cromwell's Treatise on Belts and Pulleys 12mo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, * Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. 0blong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 1 50 1 50
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 1 50 2 00
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, * Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, * Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. 0blong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 00 4 00
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. 0blong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo, Flanders's Gear-cutting Machinery. Large 12mo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 00 4 00 3 00
Barr and Wood's Kinematics of Machinery * Bartlett's Mechanical Drawing. * Abridged Ed. * Bartlett and Johnson's Engineering Descriptive Geometry. * Burr's Ancient and Modern Engineering and the Isthmian Canal. * Svo, * Burr's Heating and Ventilating Buildings. * Carpenter's Heating and Ventilating Buildings. * Carpenter and Diederichs's Experimental Engineering. * Clerk's The Gas, Petrol and Oil Engine. * Compton's First Lessons in Metal Working. * Compton and De Groodt's Speed Lathe. * Coolidge's Manual of Drawing. * Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. * Cromwell's Treatise on Belts and Pulleys. * Treatise on Toothed Gearing. * Dingey's Machinery Pattern Making. * Durley's Kinematics of Machines. * Svo, * Flanders's Gear-cutting Machinery. * Large 12mo, * Flather's Dynamometers and the Measurement of Power. * 12mo, * 12mo, * Danoge Town Town Machinery. * Large 12mo, * Flather's Dynamometers and the Measurement of Power. * 12mo, * 12mo	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 50 1 50 2 00 4 00 3 00 3 00
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. 0blong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo, Flanders's Gear-cutting Machinery. Large 12mo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 50 1 50 2 00 4 00 3 00 2 00
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing. 8vo, * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo, Compton and De Groodt's Speed Lathe 12mo, Coolidge's Manual of Drawing 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making 12mo, Durley's Kinematics of Machines 8vo, Flanders's Gear-cutting Machinery Large 12mo, Flather's Dynamometers and the Measurement of Power 12mo, Rope Driving 12mo, Gill's Gas and Fuel Analysis for Engineers 12mo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 50 1 50 2 00 4 00 3 00 3 00
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, * Clerk's The Gas, Petrol and Working. 12mo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo, Flanders's Gear-cutting Machinery. Large 12mo, Flather's Dynamometers and the Measurement of Power. 12mo, Rope Driving. 12mo, Gill's Gas and Fuel Analysis for Engineers. 12mo, Goss's Locomotive Sparks. 8vo, * Greene's Pumping Machinery. 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 2 00 4 00 3 00 2 00 1 25 2 00 4 00
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines 8vo, Flanders's Gear-cutting Machinery. Large 12mo, Flather's Dynamometers and the Measurement of Power. 12mo, Rope Driving. 12mo, Goll's Gas and Fuel Analysis for Engineers. 12mo, Goss's Locomotive Sparks. 8vo, * Greene's Pumping Machinery 8vo, Hering's Ready Reference Tables (Conversion Factors). 16mo, mor.	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 00 4 00 3 00 3 00 2 00 1 25 2 00 4 00 2 50
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo, Flanders's Gear-cutting Machinery. Large 12mo, Flather's Dynamometers and the Measurement of Power. 12mo, Rope Driving. 12mo, Goll's Gas and Fuel Analysis for Engineers. 12mo, Goss's Locomotive Sparks. 8vo, * Greene's Pumping Machinery 8vo, Hering's Ready Reference Tables (Conversion Factors). 16mo, mor. * Hobart and Ellis's High Speed Dynamo Electric Machinery. 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 00 4 00 3 00 3 00 2 00 4 00 2 50 6 00
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing 8vo, * " " Abridged Ed 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo, Compton and De Groodt's Speed Lathe 12mo, Coolidge's Manual of Drawing 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys 12mo, Treatise on Toothed Gearing 12mo, Dingey's Machinery Pattern Making 12mo, Durley's Kinematics of Machines 8vo, Flanders's Gear-cutting Machinery 12mo, Rope Driving 12mo, Gill's Gas and Fuel Analysis for Engineers 12mo, Goss's Locomotive Sparks 8vo, * Greene's Pumping Machinery 8vo, Hering's Ready Reference Tables (Conversion Factors) 16mo, mor. * Hobart and Ellis's High Speed Dynamo Electric Machinery 8vo, Hutton's Gas Engine 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 2 50 4 00 3 00 2 00 4 00 2 50 4 00 2 50 6 00 5 00
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing. 8vo, * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo, Compton and De Groodt's Speed Lathe 12mo, Coolidge's Manual of Drawing 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making 12mo, Durley's Kinematics of Machines 8vo, Flanders's Gear-cutting Machinery 12mo, Rope Driving 12mo, Goss's Locomotive Sparks 8vo, * Greene's Pumping Machinery 12mo, Hering's Ready Reference Tables (Conversion Factors) 16mo, mor. * Hobart and Ellis's High Speed Dynamo Electric Machinery 8vo, Jamison's Advanced Mechanical Drawing 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 2 50 4 00 3 00 2 00 1 25 2 00 4 00 2 50 6 00 5 00 5 00 2 00
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo, Flanders's Gear-cutting Machinery. Large 12mo, Flather's Dynamometers and the Measurement of Power. 12mo, Rope Driving. 12mo, Goll's Gas and Fuel Analysis for Engineers. 12mo, Goss's Locomotive Sparks. 8vo, * Greene's Pumping Machinery. 8vo, Hering's Ready Reference Tables (Conversion Factors), 16mo, mor. * Hobart and Ellis's High Speed Dynamo Electric Machinery 8vo, Hutton's Gas Engine. 8vo, Jamison's Advanced Mechanical Drawing. 8vo, Elements of Mechanical Drawing. 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 2 00 4 00 3 00 2 00 4 00 2 50 6 00 5 00 2 50 5 00 2 50
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working 12mo, Compton and De Groodt's Speed Lathe 12mo, Coolidge's Manual of Drawing 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo, Flanders's Gear-cutting Machinery. Large 12mo, Flather's Dynamometers and the Measurement of Power 12mo, Rope Driving. 12mo, Goss's Locomotive Sparks. 8vo, * Greene's Pumping Machinery. 8vo, Hering's Ready Reference Tables (Conversion Factors). 16mo, mor. * Hobart and Ellis's High Speed Dynamo Electric Machinery 8vo, Hutton's Gas Engine. 8vo, Jamison's Advanced Mechanical Drawing 8vo, Lements of Mechanical Drawing 8vo, Jones's Gas Engine. 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 2 50 4 00 3 00 2 00 1 25 2 00 4 00 2 50 6 00 5 00 5 00 2 00
Barr and Wood's Kinematics of Machinery. * Bartlett's Mechanical Drawing. * " " Abridged Ed. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry. 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal. 8vo, Carpenter's Heating and Ventilating Buildings. 8vo, * Carpenter and Diederichs's Experimental Engineering. 8vo, * Clerk's The Gas, Petrol and Oil Engine. 8vo, Compton's First Lessons in Metal Working. 12mo, Compton and De Groodt's Speed Lathe. 12mo, Coolidge's Manual of Drawing. 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Cromwell's Treatise on Belts and Pulleys. 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making. 12mo, Durley's Kinematics of Machines. 8vo, Flanders's Gear-cutting Machinery. Large 12mo, Flather's Dynamometers and the Measurement of Power. 12mo, Rope Driving. 12mo, Goll's Gas and Fuel Analysis for Engineers. 12mo, Goss's Locomotive Sparks. 8vo, * Greene's Pumping Machinery. 8vo, Hering's Ready Reference Tables (Conversion Factors), 16mo, mor. * Hobart and Ellis's High Speed Dynamo Electric Machinery 8vo, Hutton's Gas Engine. 8vo, Jamison's Advanced Mechanical Drawing. 8vo, Elements of Mechanical Drawing. 8vo,	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 2 00 4 00 3 00 2 00 4 00 2 50 6 00 5 00 2 50 5 00 2 50
Barr and Wood's Kinematics of Machinery 8vo, * Bartlett's Mechanical Drawing. 8vo, * Bartlett sechanical Drawing. 8vo, * Bartlett and Johnson's Engineering Descriptive Geometry 8vo, * Burr's Ancient and Modern Engineering and the Isthmian Canal 8vo, Carpenter's Heating and Ventilating Buildings 8vo, * Carpenter and Diederichs's Experimental Engineering 8vo, * Clerk's The Gas, Petrol and Oil Engine 8vo, Compton's First Lessons in Metal Working 12mo, Compton and De Groodt's Speed Lathe 12mo, Coolidge's Manual of Drawing 8vo, paper, Coolidge and Freeman's Elements of General Drafting for Mechanical Engineers. Oblong 4to, Treatise on Belts and Pulleys 12mo, Treatise on Toothed Gearing. 12mo, Dingey's Machinery Pattern Making 12mo, Durley's Kinematics of Machines 8vo, Flanders's Gear-cutting Machinery Large 12mo, Rope Driving. 12mo, Goss's Locomotive Sparks 8vo, * Greene's Pumping Machinery Hering's Ready Reference Tables (Conversion Factors) 16mo, mor. * Hobart and Ellis's High Speed Dynamo Electric Machinery 8vo, Hutton's Gas Engine 8vo, Jamison's Advanced Mechanical Drawing 8vo, Lements of Mechanical Drawing 8vo, Lements of Machineal Drawing 8vo, Lements of Mechanical Drawing 8vo, Lements	2 50 3 00 1 50 1 50 3 50 4 00 6 00 4 00 1 50 1 50 1 50 1 50 2 00 4 00 3 00 2 00 4 00 2 50 6 00 6 00 6 00 6 00 6 00 6 00 6 00 6

* Kaup's Machine Shop PracticeLarge 12mo		25
* Kent's Mechanical Engineer's Pocket-Book		00
Kerr's Power and Power Transmission		00
* King's Elements of the Mechanics of Materials and of Power of Trans-	0	00
mission8vo,	2	50
* Lanza's Dynamics of Machinery		50
Leonard's Machine Shop Tools and Methods		00
* Levin's Gas Engine		00
MacCord's Kinematics; or, Practical Mechanism		00
Mechanical Drawing		00
Velocity Diagrams		50
MacFarland's Standard Reduction Factors for Gases 8vo,		50
Mahan's Industrial Drawing. (Thompson.)		50 50
Miller, Berry, and Riley's Problems in Thermodynamics and Heat Engineer-	4	JU.
ing8vo, paper,	0	75
Oberg's Handbook of Small Tools Large 12mo,		50
* Parshall and Hobart's Electric Machine Design. Small 4to, half leather,		
* Peele's Compressed Air Plant. Second Edition, Revised and Enlarged. 8vo,		50
* Perkins's Introduction to General Thermodynamics	1 3	50 00
* Porter's Engineering Reminiscences, 1855 to 1882		00
Randall's Treatise on Heat. (In Press.)		
* Reid's Mechanical Drawing. (Elementary and Advanced.)8vo,		00
Text-book of Mechanical Drawing and Elementary Machine Design.8vo,		00
Richards's Compressed Air		50
Schwamb and Merrill's Elements of Mechanism		00
Smith (A. W.) and Marx's Machine Design		00
Smith's (O.) Press-working of Metals8vo,	3	00
Sorel's Carbureting and Combustion in Alcohol Engines. (Woodward and		-
Preston.)		50
Thurston's Animal as a Machine and Prime Motor, and the Laws of Energetics		30
12mo.		00
Treatise on Friction and Lost Work in Machinery and Mill Work8vo,	3	00
* Tillson's Complete Automobile Instructor16mo,	_	50
* Titsworth's Elements of Mechanical DrawingOblong 8vo, Warren's Elements of Machine Construction and Drawing8vo,		25 50
* Waterbury's Vest Pocket Hand-book of Mathematics for Engineers.		00
	1	00
* Enlarged Edition, Including Tables	1	50
Weisbach's Kinematics and the Power of Transmission. (Herrmann-		00
Klein.)		00
Wood's Turbines		50
MATERIALS OF ENGINEERING.		
Burr's Elasticity and Resistance of the Materials of Engineering 8vo,	7	50
Church's Mechanics of Engineering	6	00
Mechanics of Solids (Being Parts I, II, III of Mechanics of Engineering).		
* Greene's Structural Mechanics	4	50
Holley's Analysis of Paint and Varnish Products. (In Press.)	2	50
	3	00
* Lead and Zinc PigmentsLarge 12mo, Johnson's (C. M.) Rapid Methods for the Chemical Analysis of Special		
Steels, Steel-Making Alloys and Graphite Large 12mo,		00
Johnson's (J. B.) Materials of Construction		50
* King's Elements of the Mechanics of Materials and of Power of Trans-		00
mission8vo,	2	50
Lanza's Applied Mechanics		50
Lowe's Paints for Steel Structures		00
PROPERTY OF ANY ADDRESS AS A RESIDENCE OF THE COLUMN TO COMMITTED TO A STATE OF THE COLUMN TO A	-	00
14		

Maurer's Technical Mechanics	5 1 2 2 3 1 1 8 2 3	00 00 00 00 00 00 00 25 00 00 50
Wood's (De V.) Elements of Analytical Mechanics		00
Steel	4	00
STEAM-ENGINES AND BOILERS.		
Berry's Temperature-entropy Diagram. Third Edition Revised and Enlarged	2	50 50
Chase's Art of Pattern Making	2	
Creighton's Steam-engine and other Heat Motors	5	
* Gebhardt's Steam Power Plant Engineering8vo,	6	
Goss's Locomotive Performance8vo,	5	
Hemenway's Indicator Practice and Steam-engine Economy12mo, Hirshfeld and Barnard's Heat Power Engineering. (In Press.) Hutton's Heat and Heat-engines8vo,	2 5	00
Mechanical Engineering of Power Plants8vo,		00
Kent's Steam Boiler Economy		00
Kneass's Practice and Theory of the Injector		50
Meyer's Modern Locomotive Construction4to,		
Miller, Berry, and Riley's Problems in Thermodynamics8vo, paper,		75
Moyer's Steam Turbine		00 50
Entropy Table8vo,	7	00
Thermodynamics of the Steam-engine and Other Heat-engines 8vo, * Thermodynamics of the Steam Turbine		00
Valve-gears for Steam-engines8vo,		50
Peabody and Miller's Steam-boilers		00
Pupin's Thermodynamics of Reversible Cycles in Gases and Saturated Vapors. (Osterberg.)		50 25
Reagan's Locomotives: Simple, Compound, and Electric. New Edition.		
Sinclair's Locomotive Engine Running and Management12mo,		50
Smart's Handbook of Engineering Laboratory Practice		50
Snow's Steam-boiler Practice8vo,		00
Spangler's Notes on Thermodynamics		00 50
Spangler, Greene, and Marshall's Elements of Steam-engineering 8vo,		00
Thomas's Steam-turbines	4	00
Thurston's Handbook of Engine and Boiler Trials, and the Use of the Indicator and the Prony Brake	5	00
Handy Tables8vo,	1	50
Manual of Steam-b, Yers, their Designs, Construction, and Operation 8vo, Manual of the Steam-engine		00
Part I. History, Structure, and Theory		00
Part II. Design, Construction, and Operation8vo,		00

Wehrenfennig's Analysis and Softening of Boiler Feed-water. (Patterson.)		
Weisbach's Heat, Steam, and Steam-engines. (Du Bois.)	5 (00
	4 (JU
MECHANICS PURE AND APPLIED.		
Church's Mechanics of Engineering	6 (3 (1 5	00
Notes and Examples in Mechanics	2 0	
Dana's Text-book of Elementary Mechanics for Colleges and Schools .12mo, Du Bois's Elementary Principles of Mechanics:	1.5	50
Vol. I. Kinematics	3 5	
Mechanics of Engineering. Vol. ISmall 4to,	7 5	50
Vol. II		
* Greene's Structural Mechanics	2 5 1 2	
* Johnson's (W. W.) Theoretical Machanias	2 0	
* Johnson's (W. W.) Theoretical Mechanics	3 0	10
mission8vo,	2 5	
Lanza's Applied Mechanics	7 5 1 2	
* Vol. II. Kinematics and Kinetics	1 5	
* Vol. III. Mechanics of Materials	1 5	
* Merriman's Elements of Mechanics	4 0 1 0	
Mechanics of Materials8vo,	5 0	
* Michie's Elements of Analytical Mechanics	4 0 3 0	
Sanborn's Mechanics Problems Large 12mo,	1 5	
Schwamb and Merrill's Elements of Mechanism	3 0	
Principles of Elementary Mechanics	$\frac{3}{1} \frac{0}{2}$	
MEDICAL.		
*Abderhalden's Physiological Chemistry in Thirty Lectures. (Hall and	- 0	-
Defren.)	5 0	
* Bolduan's Immune Sera	1 5	0
Bordet's Studies in Immunity. (Gay.)	6 0	
Davenport's Statistical Methods with Special Reference to Biological Variations	1 5	
Ehrlich's Collected Studies on Immunity. (Bolduan.)	6 0	
*Fischer's Nephritis	2 50	
* Physiology of AlimentationLarge 12mo,	2 0	0
* de Fursac's Manual of Psychiatry. (Rosanoff and Collins.)Large 12mo, *Hammarsten's Text-book on Physiological Chemistry. (Mandel.)8vo,	2 50	
Jackson's Directions for Laboratory Work in Physiological Chemistry 8vo.	1 2	5
Lassar-Cohn's Praxis of Urinary Analysis. (Lorenz.)	1 00	
* Nelson's Analysis of Drugs and Medicines	3 00	
* Pauli's Physical Chemistry in the Service of Medicine. (Fischer.)12mo,	1 2	
* Pozzi-Escot's Toxins and Venoms and their Antibodies. (Cohn.). 12mo, Rostoski's Serum Diagnosis. (Bolduan.)	1 00	
Ruddiman's Incompatibilities in Prescriptions8vo,	2 00	0
Whys in Pharmacy	2 50	
The state of the s	- 01	-


* Satterlee's Outlines of Human Embryology	81	25
Smith's Lecture Notes on Chemistry for Dental Students8vo,		50
* Whipple's Tyhpoid FeverLarge 12mo,		000
* Woodhull's Military Hygiene for Officers of the Line Large 12mo,	1	50
* Personal Hygiene	1	00
Worcester and Atkinson's Small Hospitals Establishment and Maintenance,	-	
and Suggestions for Hospital Architecture, with Plans for a Small		
Hospital12mo,	1	25
METALLIDAY		
METALLURGY.		*
Betts's Lead Refining by Electrolysis8vo,	4	00
Bolland's Encyclopedia of Founding and Dictionary of Foundry Terms used		
	-	nn
in the Practice of Moulding		00
Iron Founder	2	50
" " Supplement12mo,	2	50
* Borchers's Metallurgy. (Hall and Hayward.)8vo,		00
	0	00
* Burgess and Le Chatelier's Measurement of High Temperatures. Third		
Edition	4	00
Edition	1	00
Goesel's Minerals and Metals: A Reference Book16mo, mor.		00
* Iles's Lead-smelting	2	50
Johnson's Rapid Methods for the Chemical Analysis of Special Steels,		
Steel-making Alloys and Graphite Large 12mo,	3	GO
		50
Keep's Cast Iron		
Metcalf's Steel. A Manual for Steel-users		00
Minet's Production of Aluminum and its Industrial Use. (Waldo.) 12mo,	2	50
* Palmer's Foundry PracticeLarge 12mo,		00
* Price and Meade's Technical Analysis of Brass		00
* Ruer's Elements of Metallography. (Mathewson.)8vo,	3	00
Smith's Materials of Machines	1	00
Tate and Stone's Foundry Practice12mo,		00
Thurston's Materials of Engineering. In Three Parts8vo,	8	00
Part I. Non-metallic Materials of Engineering, see Civil Engineering,		
page 9.		
Part II. Iron and Steel8vo,	2	50
Part II. If and Steel.	0	00
Part III. A Treatise on Brasses, Bronzes, and Other Alloys and their		
Constituents8vo,	2	50
Ulke's Modern Electrolytic Copper Refining8vo,	3	00
West's American Foundry Practice	2	
Moulders' Text Book	-	50
MINERALOGY.		
* Promping's Introduction to the Poses Flowerts	1	50
* Browning's Introduction to the Rarer Elements8vo,		50
Brush's Manual of Determinative Mineralogy. (Penfield.)8vo,	4	00
Butler's Pocket Hand-book of Minerals	3	00
Chester's Catalogue of Minerals8vo, paper,		00
Cloth,		25
* Crane's Gold and Silver8vo,		00
Dana's First Appendix to Dana's New "System of Mineralogy" Large 8vo,	1	00
Dana's Second Appendix to Dana's New "System of Mineralogy."		
	7	50
Large 8vo,		
Manual of Mineralogy and Petrography12mo,		00
Minerals and How to Study Them	1	50
System of MineralogyLarge 8vo, half leather,	12	50
Text-book of Mineralogy		00
		00
Dougloc's Intochnical Addresses on Technical Colorects		
Douglas's Untechnical Addresses on Technical Subjects		
Eakle's Mineral Tables8vo,	1	
Eakle's Mineral Tables8vo,	1	25
Eakle's Mineral Tables	1 3	00
* Eckel's Building Stones and Clays	1 3 3	00
* Eckel's Building Stones and Clays	1 3 3 3	00 00 50
* Eckel's Building Stones and Clays	1 3 3 3 1	00 00 50 25
* Eckel's Building Stones and Clays	1 3 3 3 1	00 00 50
* Eckel's Building Stones and Clays	1 3 3 1 1	00 00 50 25 50
* Eckel's Building Stones and Clays	1 3 3 1 1 5	00 00 50 25 50 00
* Eckel's Building Stones and Clays	1 3 3 1 1 5	00 00 50 25 50


Johannsen's Determination of Rock-forming Minerals in Thin Sections. 8vo,	
* Martin's Laboratory Guide to Qualitative Analysis with the Blow-	
pipe	0 60
Stones for Building and Decoration8vo.	5 00
* Penfield's Notes on Determinative Mineralogy and Record of Mineral Tests.	
8vo, paper,	0 50
Tables of Minerals, Including the Use of Minerals and Statistics of Domestic Production	1 00
* Pirsson's Rocks and Rock Minerals	1 00 2 50
* Richards's Synopsis of Mineral Characters	1 25
* Ries's Clays: Their Occurrence, Properties and Uses8vo,	5 00
* Ries and Leighton's History of the Clay-working inqustry of the United	
States	2 50 1 25
* Tillman's Text-book of Important Minerals and Rocks	2 00
Washington's Manual of the Chemical Analysis of Rocks8vo,	2 00
MINING.	
* Beard's Mine Gases and Explosions Large 12mo,	3 00
* Crane's Gold and Silver	5 0.0
* Index of Mining Engineering Literature8vo, * 8vo, mor.	4 00 5 00
* Ore Mining Methods8vo,	3 00
* Dana and Saunders's Rock Drilling8vo,	4 00
Douglas's Untechnical Addresses on Technical Subjects	1 00
Eissler's Modern High Explosives8vo,	4 00
Goesel's Minerals and Metals: A Reference Book16mo, mor.	3 00
Ihlseng's Manual of Mining	5 00 2 50
* Peele's Compressed Air Plant8vo,	3 50
Riemer's Shaft Sinking Under Difficult Conditions. (Corning and Peele.)8vo,	3 00
* Weaver's Military Explosives	3 00
Wilson's Hydraulic and Placer Mining. 2d edition, rewritten12mo, Treatise on Practical and Theoretical Mine Ventilation12mo,	2 50 1 25
Treatise on Tractical and Theoretical Name Ventilation	1 20
SANITARY SCIENCE.	
Association of State and National Food and Dairy Departments, .Hartford	
Meeting, 1906	3 00
Jamestown Meeting, 1907	3 00 1 25
Sanitation of a Country House	1 00
Sanitation of Recreation Camps and Parks12mo,	1 00
* Chapin's The Sources and Modes of InfectionLarge 12mo,	3 00
Folwell's Sewerage. (Designing, Construction, and Maintenance.)8vo,	3 00
Water-supply Engineering	4 00 2 00
Fuertes's Water-filtration Works	2 50
Water and Public Health	1 50
Gerhard's Guide to Sanitary Inspections	1 50
* Modern Baths and Bath Houses	3 00 1 50
Sanitation of Public Buildings	1 30
8vo,	4 00
Hazen's Clean Water and How to Get It Large 12mo,	1 50
Filtration of Public Water-supplies	3 00
* Kinnicutt, Winslow and Pratt's Sewage Disposal	3 00
Control8vo,	7 50
Mason's Examination of Water. (Chemical and Bacteriological)12mo,	1 25
Water-supply. (Considered principally from a Sanitary Standpoint).	
* Most's Light and the Rehavior of Organisms Large 12mo	4 00 2 50
* Mast's Light and the Behavior of OrganismsLarge 12mo,	2 00

* Merriman's Elements of Sanitary Engineering 8vo,		
Ogden's Sewer Construction8vo,	3 (
Sewer Design	2	
Parsons's Disposal of Municipal Refuse	2	00
Prescott and Winslow's Elements of Water Bacteriology, with Special Refer-	1	-0
ence to Sanitary Water Analysis		50
* Price's Handbook on Sanitation	1 .	50
Cost of Cleanness	1	
Cost of Food. A Study in Dietaries		00
Cost of Living as Modified by Sanitary Science		00
Cost of Shelter		00
Richards and Woodman's Air, Water, and Food from a Sanitary Stand-	-	00
	2 (00
* Richey's Plumbers', Steam-fitters', and Tinners' Edition (Building	100	
Mechanics' Ready Reference Series) 16mo, mor.	1	50
Rideal's Disinfection and the Preservation of Food8vo,	4	00
Soper's Air and Ventilation of Subways	2	50
Turneaure and Russell's Public Water-supplies 8vo,	5	00
Venable's Garbage Crematories in America8vo.	2	00
Method and Devices for Bacterial Treatment of Sewage 8vo,	3	00
Ward and Whipple's Freshwater Biology. (In Press.)		
Whipple's Microscopy of Drinking-water8vo,	3	
* Typhoid Fever	3	
Value of Pure Water	1	
Winslow's Systematic Relationship of the CoccaceæLarge 12mo,	2	50
MISCELLANEOUS.		
MICOLD DINIDOCCI		
* Burt's Railway Station Service	2	
* Chapin's How to Enamel	1	00
Emmons's Geological Guide-book of the Rocky Mountain Excursion of the		22
International Congress of Geologists Large 8vo,		50
Ferrel's Popular Treatise on the Winds8vo,	4	
Fitzgerald's Boscon Machinist18mo,	1	
* Fritz, Autobiography of John		00
Gannett's Statistical Abstract of the World	0	
Haines's American Railway Management		50
Jacobs's Betterment Briefs. A Collection of Published Papers on Or-	3	00
ganized Industrial Efficiency8vo,	2	50
Metcalfe's Cost of Manufactures, and the Administration of Workshops8vo.		00
* Parkhurst's Applied Methods of Scientific Management8vo.		00
Putnam's Nautical Charts		00
Ricketts's History of Rensselaer Polytechnic Institute 1824-1894.		
Large 12mo,	3	00
* Rotch and Palmer's Charts of the Atmosphere for Aeronauts and Aviators.		
Oblong 4to,	2	00
Rotherham's Emphasised New TestamentLarge 8vo,	2	00
Rust's Ex-Meridian Altitude, Azimuth and Star-finding Tables8vo	5	00
Standage's Decoration of Wood, Glass, Metal, etc		00
Thome's Structural and Physiological Botany. (Bennett)16mo,		25
Westermaier's Compendium of General Botany. (Schneider)8vo,		00
Winslow's Elements of Applied Microscopy12mo,	1	50
HEBREW AND CHALDEE TEXT-BOOKS.		
Gesenius's Hebrew and Chaldee Lexicon to the Old Testament Scriptures.	1	20
(Tregelles.)Small 4to, half mor,		00
Green's Elementary Hebrew Grammar12mo	1	25





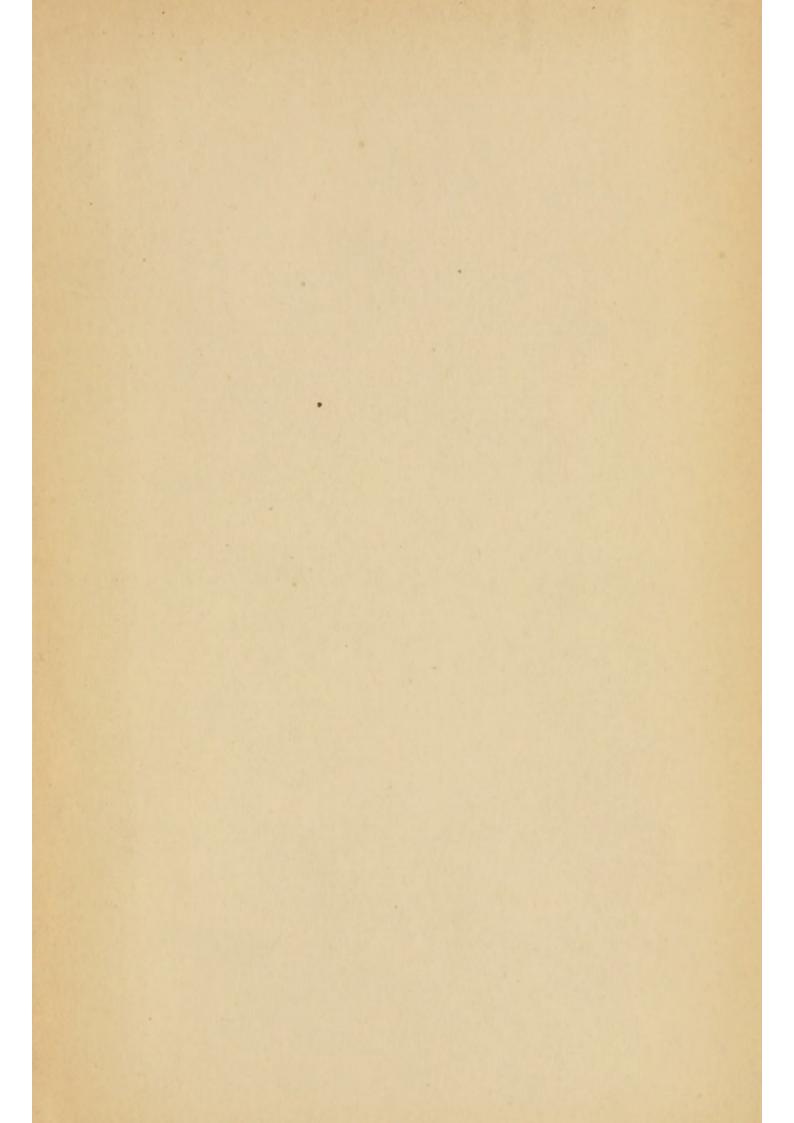

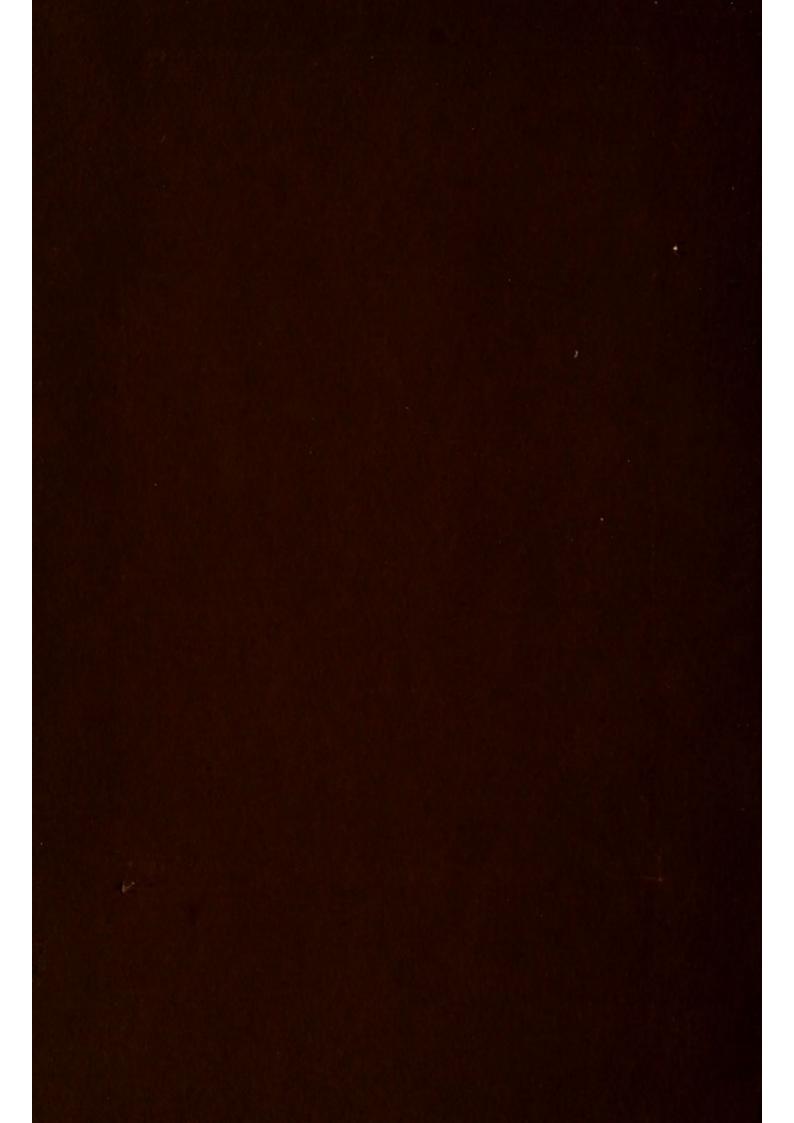

QP341 Marrin Induction Shocks 7-20-36

