

M0003686: Apparatus for nitrous oxide oxygen and ether shown by F.E. Shipway M.D.

Publication/Creation

November 1933

Persistent URL

<https://wellcomecollection.org/works/ug2r4dk2>

License and attribution


Conditions of use: it is possible this item is protected by copyright and/or related rights. You are free to use this item in any way that is permitted by the copyright and related rights legislation that applies to your use. For other uses you need to obtain permission from the rights-holder(s).

**wellcome
collection**

Wellcome Collection
183 Euston Road
London NW1 2BE UK
T +44 (0)20 7611 8722
E library@wellcomecollection.org
<https://wellcomecollection.org>

hand-key. Long levers are used for regulating the flow of the gases; should the valves be tight at first opening, the cylinders should be steadied with the hand. A spirit lamp, to keep the valves of the N_2O cylinders from freezing, can be used with either the vertical or horizontal pattern.

For hospital use, the construction of the stand is slightly modified.

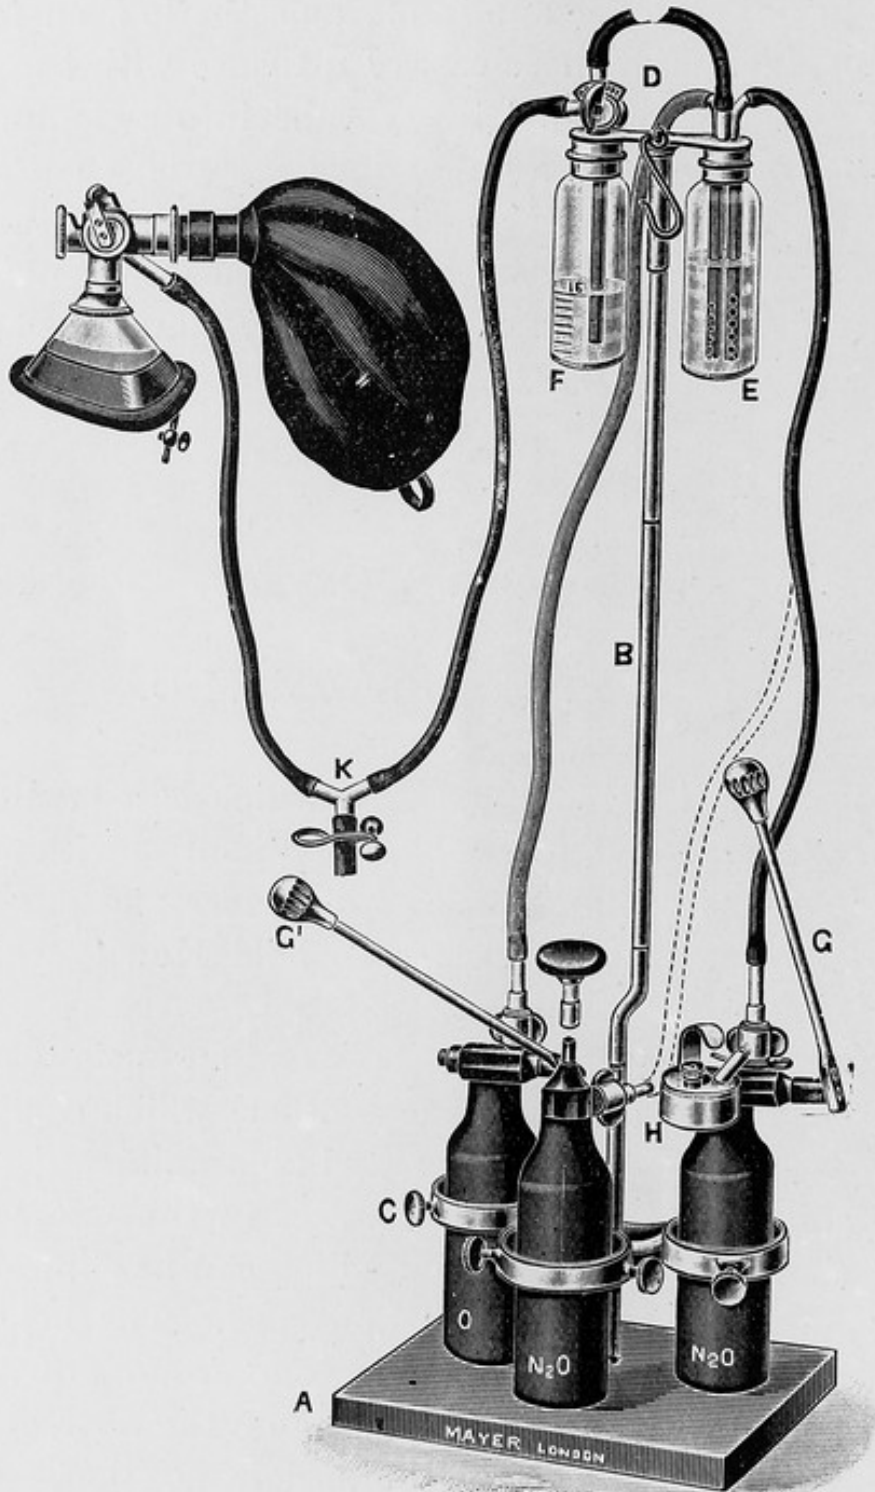

A, wooden base; B, upright rod; C, holder for cylinders; D, unit; E, mixing chamber; F, ether bottle; G, G, levers; H, spirit lamp; K, water-trap.